



## New Flagship



# Electrical Safety Multi-analyzer TOS9300 Series

All-in-one safety tester model (TOS9303LC)

Insulation diagnosis available with partial discharge model (TOS9301PD <NEW>)

New amplifier type allows for 40 A AC/DC ground bond testing (Ground bond tester models)

Electrical breakdown inspection setting available

AC5 kV/100 mA, DC7.2 kV/100 W Hipot test

Touch current/protective conductor current/leakage current test (TOS9303LC)

LAN/USB/RS232C standard digital interface

Easy to read LCD display for real time monitoring during tests

All measurement values and standard outlines displayed in each test

High voltage scanner capable of output distribution both standalone and when connected with existing



# THE ALL-ROUN

Hipot, Insulation Resistance, Ground Bond, Leakage or Partial Discharge, this analyzer covers it all!

## TOS9300 Series Lineup

### TOS9300

AC Hipot Tester with Insulation Resistance Test

ACW 5 kV/100 mA(500 VA)  
IR 0.001 M $\Omega$  to 100.0 G $\Omega$  (DC-25 V to -1000 V)  
Rise Time Fall Time LAN USB RS232C Timer



D 430(16.93" )(440(17.32" ))W×132(5.2" )(155(6.10" ))H×  
370(14.57" )(410(16.14" ))Dmm (inch)  
W Approx.17 kg(37.5 lbs)

### TOS9301

AC/DC Hipot Tester with Insulation Resistance Test

ACW 5 kV/100 mA(500 VA)  
DCW 5 kV/20 mA, 7.2 kV/13.9 mA(100 W)  
IR 0.001 M $\Omega$  to 100.0 G $\Omega$  (DC-25 V to -1000 V/DC+50 V to +7200 V)  
Rise Time Fall Time LAN USB RS232C Timer



D 430(16.93" )(440(17.32" ))W×132(5.2" )(155(6.10" ))H×  
370(14.57" )(410(16.14" ))Dmm (inch)  
W Approx.18 kg(39.7 lbs)

### TOS9301PD

NEW

AC/DC Hipot Tester with Insulation Resistance and Partial Discharge Test

ACW 5 kV/100 mA(500 VA)  
DCW 5 kV/20 mA, 7.2 kV/13.9 mA(100 W)  
IR 0.001 M $\Omega$  to 100.0 G $\Omega$  (DC-25 V to -1000 V/DC+50 V to +7200 V)  
PD 5 kV/50 mA(250 VA)  
Rise Time Fall Time LAN USB RS232C Timer



D 430(16.93" )(440(17.32" ))W×132(5.2" )(150(5.9" ))H×  
525(20.67" )(565(22.24" ))Dmm (inch)  
W Approx.22 kg(48.5 lbs)

### TOS9302

AC Hipot Tester with Ground Bond Test

ACW 5 kV/100 mA(500 VA)  
EC 0.001  $\Omega$  to 0.600  $\Omega$  (3.0 A to 42.0 A)  
Rise Time Fall Time LAN USB RS232C Timer



D 430(16.93" )(440(17.32" ))W×132(5.2" )(155(6.10" ))H×  
500(19.69" )(540(21.26" ))Dmm (inch)  
W Approx.20 kg(44.1 lbs)

### TOS9303

AC/DC Hipot Tester with Insulation Resistance and Ground Bond Test

ACW 5 kV/100 mA(500 VA)  
DCW 5 kV/20 mA, 7.2 kV/13.9 mA(100 W)  
IR 0.001 M $\Omega$  to 100.0 G $\Omega$  (DC-25 V to -1000 V/DC+50 V to +7200 V)  
EC 0.001  $\Omega$  to 0.600  $\Omega$  (3.0 A to 42.0 A)  
Rise Time Fall Time LAN USB RS232C Timer



D 430(16.93" )(440(17.32" ))W×132(5.2" )(155(6.10" ))H×  
500(19.69" )(540(21.26" ))Dmm (inch)  
W Approx.21 kg(46.3 lbs)

### TOS9303LC

AC/DC Hipot Tester with Insulation Resistance, Ground Bond, and Leakage Current Test

ACW 5 kV/100 mA(500 VA)  
DCW 5 kV/20 mA, 7.2 kV/13.9 mA(100 W)  
IR 0.001 M $\Omega$  to 100.0 G $\Omega$  (DC-25 V to -1000 V/DC+50 V to +7200 V)  
EC 0.001  $\Omega$  to 0.600  $\Omega$  (3.0 A to 42.0 A)  
LC 1  $\mu$ A to 100 mA(rms)  
Rise Time Fall Time LAN USB RS232C Timer



D 430(16.93" )(440(17.32" ))W×132(5.2" )(155(6.10" ))H×  
500(19.69" )(550(21.65" ))Dmm (inch)  
W Approx.22 kg(48.5 lbs)

## ● Test items

Model	AC Withstanding Voltage (AC Hipot)	DC Withstanding Voltage (DC Hipot)	Insulation Resistance	Earth Continuity (Ground Bond)	Leakage Current	Partial Discharge
TOS9300	●		●			
TOS9301	●	●	●			
TOS9301PD <b>NEW</b>	●	●	●			●
TOS9302	●			●		
TOS9303	●	●	●	●		
TOS9303LC	●	●	●	●	●	

# DER



**SAFETY ANALYZER**  
**TOS9300**  
**SERIES**

## Electrical Safety Multi-analyzer TOS9300 Series

The TOS9300 series is a high-performance electrical safety analyzer that complies with a wide range of universal standards. Hipot, Insulation Resistance, Ground Bond, Leakage Current (touch current and protective conductor current) and partial discharge can all be tested. A total of 6 models are available for standard compliance tests for a wide variety of applications including R&D, quality assurance manufacturing lines and laboratory tests.

- All-in-one safety tester model (TOS9303LC)
  - Insulation diagnosis available with partial discharge model (TOS9301PD [NEW])
  - New amplifier type allows for 40A AC/DC ground bond testing (Ground bond tester models)
  - Electrical breakdown inspection setting available
  - AC5 kV/100 mA, DC7.2 kV/100 W Hipot test
  - Touch current/protective conductor current/leakage current testing (TOS9303LC)
  - LAN/USB/RS232C standard digital interface
  - Easy-to-read LCD display for real-time monitoring during tests.
- All measurement values and standards outlines are displayed during each test
- High voltage scanner capable of output distribution both standalone and when connected with existing withstanding voltage/insulation resistance testing equipment models [TOS5300 series, etc.] (TOS9320)

### Option

## TOS9320

### High-voltage Scanner

High-voltage scanner for TOS9300 series multi-channel testing systems



CE UK CA

**D** 430(16.93" )(440(17.32" ))W×88(3.46" )(105(4.13" ))H×  
370(14.57" )(390(15.35" ))Dmm(inch)  
**W** Approx. 8 kg (17.6 lbs)

### Others



Remote control box  
High-voltage test probe  
Test probe for touch current test  
Warning light unit  
Multi outlet  
DIN conversion cable  
Rack mount bracket

### Features

P4-P7

### Applications

P8-9

### Exterior Design

P10-11

### Specifications

P12-P26

### Dimensions

P27

### Option/Other

P28-P29

<b>ACW</b> Max. output-voltage of AC hipot testing	<b>Rise Time</b> Equipped with rise time control function	<b>D</b> Dimensions(maximum)
<b>DCW</b> Max. output-voltage of DC hipot testing	<b>Fall Time</b> Equipped with fall time control function	<b>W</b> Weight
<b>IR</b> Measurement range of insulation resistance testing	<b>LAN</b> Equipped with LAN interface as standard	<b>Timer</b> Equipped with timer function
<b>EC</b> Measurement range of ground bond testing	<b>USB</b> Equipped with USB interface as standard	
<b>LC</b> Measurement range of leakage current testing	<b>RS232C</b> Equipped with RS232C interface as standard	
<b>PD</b> Measurement range of partial discharge testing		

The Electrical Appliance & Material Safety Low (Japan), UL (U.S.A.), CSA (Canada), VDE (Germany) and BS (U.K.) are some major examples of safety standards in use throughout the world that require the performing of hipot testing. For this reason, it is necessary to confirm for what portion of what standard testing is to be performed when purchasing a hipot tester. Although the 500 VA capacity hipot testers available from KIKUSUI can basically be applied to tests specified in all safety standards, we recommend that you consult with us prior to purchase in order to select the model that best matches your specific application.


For the withstanding test and the insulation resistance test of the EUT (equipment under test) with turned on electricity.

Our hipot testers and insulation resistance testers are designed to test the EUT(equipment under test) with the electricity turned off. In case the test requires the EUT(equipment under test)

# Features

## Color LCD Screen for Improved Visibility!

A brand-new, 7-inch LCD display allows for easy access to your custom settings, standard outlines and blueprints for easy operation. (See Exterior Design P10/Display P11)

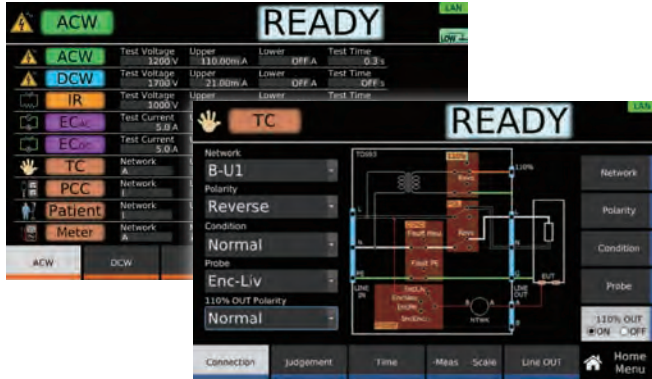

## User-Friendly, 10-Key Configuration

The TOS9300 series has included a user-friendly keypad in addition to the basic rotary knob for easy configuration setting. The front panel USB interface also allows for direct control via keyboard\*.



\*106/109 Japanese keyboards and 101/104 English keyboard compliant.

## Easy Firmware Updates via USB

System firmware can easily be updated via USB memory with updated files directly accessible from our website. (<https://www.kikusui.co.jp/en/download/>)



## LAN/USB/RS232C Standard Digital Interface

LXI compatible LAN, USB 2.0, USB-TMC compatible USB, and RS232C as standard digital interface.



▲Rear panel, Interface(All models)

◀ Use a browser from a PC, smartphone, or tablet to access the web server built into the TOS9300 series for convenient control and monitoring.


[Recommended browser]

- Requires for the Internet Explorer version 9.0 or later
- Requires for the firefox 8.0 or later
- Requires for the safari / mobile Safari 5.1 or later
- Requires for the Chrome 15.0 or later

\* Connecting with a smartphone, tablet, etc. requires a Wi-Fi environment (wireless LAN)

## I/V Monitor Terminal (Analog Monitor)

Signal outputs on the rear panel I/V terminal allow the user to monitor current/voltage waveforms during hipot tests with only an oscilloscope. Current sensors and high-voltage probes are not required.

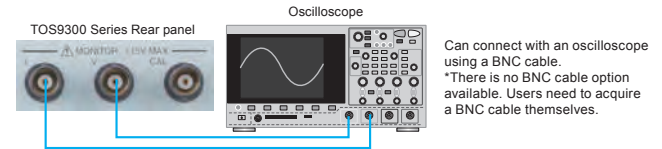

## STATUS OUT Connector


Signals from the rear panel STATUS connector automatically activate the optional warning light (PL02-TOS) during high voltage output or unsafe test conditions.



## SIGNAL I/O Connector

The rear panel also has a SIGNAL I/O that can start/stop operation as well as output signals.

TOS9300 example (The SIGNAL I/O connector is the same on all models.)

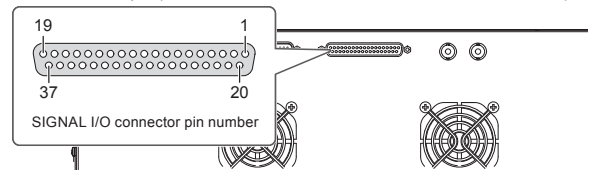

Pin no.	IN/OUT	Signal name	Description
1	—	INTERLOCK+	Activate/release interlock.
2	—	COM	Circuit common (chassis potential) shared by input and output.
3	IN	PM0	Select setup memories and auto test program memories.
4	IN	PM1	
5	IN	PM2	
6	IN	PM3	
7	IN	PM4	
8	IN	PM5	
9	IN	PM6	
10	IN	PM7	
11	IN	STB	Recall setup memories and programs selected with the PM0 to PM7 signals.
12	—	Reserved	Not used.
13	—	Reserved	
14	—	Reserved	
15	IN	START	Start a test.
16	IN	STOP	Stop a test.
17	IN	ENABLE	Enable the START signal.
18	—	COM	I/O circuit common (chassis potential).
19	IN	INTERLOCK-	Activate/release interlock.
20	—	COM	I/O circuit common (chassis potential).
21	—	+24V	+24 V internal power supply output terminal. Maximum output current 100 mA.
22	OUT	H.V ON/LINE ON	Set to on in any of the following conditions. Testing, Auto testing. Voltage remaining across the output terminals. Power being supplied to the EUT from the TOS9303LC through AC LINE OUT.
23	OUT	RISE	Set to on when the voltage is rising.
24	OUT	TEST	Set to on during test time.
25	OUT	PASS	Set to on for the duration of time specified by Pass Hold when a PASS judgment is made.
26	OUT	U FAIL	Set to on continuously when a U-FAIL judgment is made. Or set to on continuously along with the L FAIL signal when CONTACT FAIL judgment is made when a scanner is connected.
27	OUT	L FAIL	Set to on continuously when an L-FAIL judgment is made. Or set to on continuously along with the U FAIL signal when CONTACT FAIL judgment is made when a scanner is connected.
28	—	Reserved	Not used.
29	OUT	READY	Set to on when the product is ready to start a test.
30	OUT	PROTECTION	Set to on when a protection function is activated.
31	OUT	STEP END	Set to on when each step ends during an auto test.
32	OUT	CYCLE END	Set to on when the last step ends during an auto test.
33	OUT	ACW	Set to on when the test mode is set to AC withstanding voltage test.
34	OUT	DCW	Set to on when the test mode is set to DC withstanding voltage test.
35	OUT	IR	Set to on when the test mode is set to insulation resistance test.
36	OUT	EC	Set to on when the test mode is set to earth continuity test.
37	—	Reserved	Set to on when the test mode is set to touch current test or



## Universal Input Support

### ● Global Support

TOS9300 Series supports universal input for varying input voltages around the world.




### ● Programmable Output Frequency

Stable output frequency not dependent on input power source. Testing voltage is supplied at a stable 50/60Hz frequency.



## AC Hipot Testing with Stable Output [Input Voltage Variation: $\pm 0.3\%$ ]

Conventional hipot testers utilize a slide transformer to output AC line voltage. This design is susceptible to input voltage fluctuation, with outside electrical influence affecting the test results. This can result in distorted voltage being applied to the EUT which can cause product malfunctions down the line due to component malfunction. The TOS9300 series utilizes a highly efficient PWM amplifier capable of stable high-voltage output that is unaffected by changes in the AC power line. The TOS9300 series allows for safe, stable, and highly reliable tests regardless of AC power line instability.

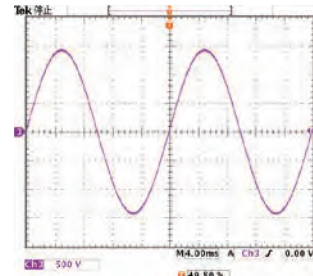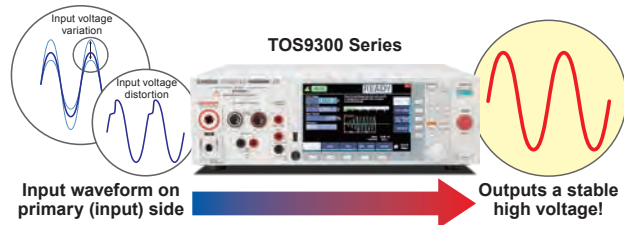

## High Precision/High Resolution/High Speed

The TOS9300 is equipped with a highly accurate, high resolution RMS measurement circuit with a voltmeter of  $\pm (1.2\%$  of reading  $+5\text{ V})$ /minimum resolution  $0.1\text{ V}$  and an ammeter of  $\pm (1\%$  of reading  $+2\text{ }\mu\text{A})$ / minimum resolution  $1\text{ }\mu\text{A}$ . The series also supports an auto range function, ensuring similar accuracy in both the upper and lower limit measurements that can accurately detect connection problems in the test lead. This, combined with a measurement speed of  $0.1\text{ s}$ , allows for reliable testing with high accuracy and resolution.

## Supports testing for partial discharge (TOS9301PD)


By observing minute partial discharges, it is possible to detect deterioration inside the insulation and "potential defects" that can affect the life of the insulation, which cannot be detected by the withstand voltage test. (See Application P9 and Specification P18)



## Automatic Testing Feature

Tests can be combined and configured to execute automatically over long periods of time. Automatic tests are composed of programs and steps, which can be configured to initiate one after another.

### ● Program schematic



	Maximum number of programs	Maximum number of steps *1	Executed under external control	Changing the program name
Program memory (except LC tests)	100	100	—	✓
Program memory (LC tests only) *2	100	100	—	✓


  

	Maximum number of programs	Maximum number of steps *1	Executed under external control	Changing the program name
External control program memory (except LC tests)	25	100	✓	—
External control Program memory (LC tests only) *2	24	100	✓	—

\*1 Per program \*2 TOS9303LC only

## Contact/Protective Conductor/ Patient Leakage Current Test (TOS9303LC)

The TOS9300 series can conduct leakage current (patient current) tests for highly sensitive medical devices. Measurement networks can be easily configured via the front panel. (See Applications P8, Specifications P21)

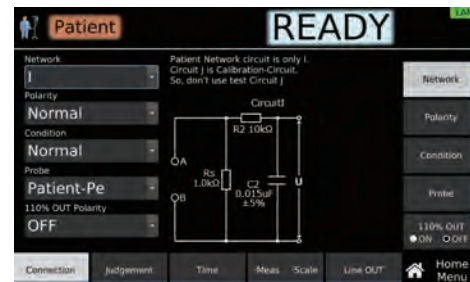

## All Electrical Safety Standard Tests in One Device! (TOS9303LC)

The TOS9303LC is the "all-rounder" model that supports AC/DC withstanding voltage, insulation resistance, AC/DC earth continuity and leakage currents tests in a single device. It can also be used for contact current, protective conductor current and patient leakage current tests.

ACW	5 kV/100 mA(500 VA)
DCW	5 kV/20 mA, 7.2 kV/13.9 mA(100 W)
IR	0.001 M $\Omega$ to 100.0 G $\Omega$ (DC-25 V to -1000 V/DC+50 V to +7200 V)
EC	0.001 $\Omega$ to 0.600 $\Omega$ (3.0 A to 42.0 A)
LC	1 $\mu\text{A}$ to 100 mA(rms)

*All in One!*



# Features

## Programmable Detection Response Speed

Conventional withstanding voltage testers are generally used to only detect insulation breakdown, and cannot make judgements on instantaneous discharge currents like partial discharge. However, the TOS9300 series is equipped with 5 levels of response speed settings to accurately detect low levels of insulation breakdown. Small discharges not visible to conventional withstanding voltage testers are easily detected with the TOS9300 series.

Value	Description
LPF	<b>Slow</b> Mean value response type current detector. This is similar to the current detection response of Kikusui's general-purpose AC withstanding voltage testers. This setting is suitable for detecting dielectric breakdown defined in safety standards and for general hipot tests for general electronic devices and components. This setting is not recommended for detecting corona discharge, which is not considered dielectric breakdown by typical safety standards.
	<b>Medium</b> Mean value response type is faster than the SLOW setting. Upper limit judgement detection is much faster, suitable for withstanding voltage tests on compact electronic components and other EUTs prone to dielectric breakdown. Instantaneous discharges such as corona discharges with high frequencies are detected which may not be suitable for simple withstanding voltage tests.
	<b>Fast</b> Extremely small discharges such as corona discharges are detected but with low reproducibility.
HPF	<b>Slow</b>
	<b>Fast</b>



## 7.2 kV/100 W DC Hipot Test

Capable of performing DC Hipot tests up to 7.2 kV utilizing a stable DC/DC converter with low-ripple and load variation of 1% and below.



## Positive Electrode/Negative Electrode Insulation Resistance Testing

Testing voltage from -25 V to -1000 V, +50 V to +7200 V, with a setting resolution is 1 V. Insulation resistance can be tested up to 99.99 GΩ. This makes for easy IEC61730-2 standard PV (solar battery) module insulation resistance testing. (See Application P9)



## Electric Discharge Function

A discharge feature enables discharge of electrical energy from the DUT after DC hipot and insulation resistance tests have been completed. The setting range for discharge time is between 0.0s - 100.0s.


## AC/DC Earth Continuity Testing up to 40 A

Cutting edge amp technology allows for a wide range of applications, including general AC earth conduction testing and EV/PHV system DC earth continuity testing. This also allows for strict adherence to automotive DC standard requirements, which are expected to increase in the near future.



## EARTH FAULT Protection

Mistakenly changing the grounding (GND) setting to "guard" (floating) can result in grounding the test subject which can result in unwanted leakage current emissions from the high voltage output site into the grounding site, resulting in electric shock to the operator. The EARTH FAULT protection function blocks output and terminates the test; eliminating any risk of electric shock and maximizing safety for the operator.

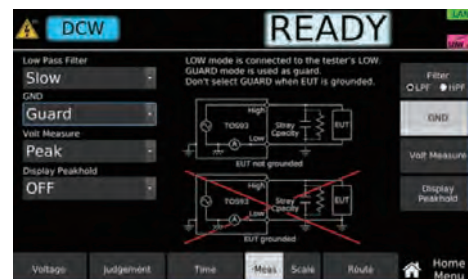


## Offset Cancel

The Offset Cancel feature allows the user to eliminate electrical current found in the insulation resistance and stray capacitance among the output cables (only resistance for DC testing). This feature is available in all testing modes for AC withstanding voltage, DC withstanding voltage, insulation resistance, earth continuity and electrical current leakage tests.

## Rise Time/Fall Time Control Function


The rise time control function prevents unnecessary stress from being applied to the EUT.

### ● Rise Time control function

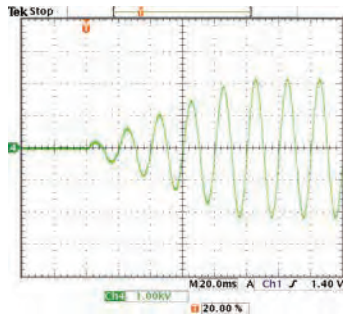

The rise time control feature allows you to gradually increase voltage to a set value while AC/DC hipot tests are conducted. Voltage rise times can be set from 0.1s to 200.0s at a resolution of 0.1s.

### ● Fall time control function

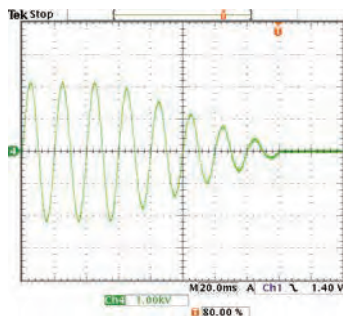

The fall time control feature allows you to gradually decrease the test voltage after a successful AC/DC hipot test. The voltage fall time can be set from 0s to 200s at a resolution of 0.1s. (OFF is also selectable).

## Basic Memory Function

In addition to automatic testing memory functions, up to 51 basic setting conditions and testing modes can be selected and saved to the main unit or USB memory. Easy testing with no hassle!

"sda1" is the folder displayed when USB memory is inserted.



Testing conditions can be saved in 00-50 of "setups". (Total 51)

## Calibration Deadline Notification

A real-time clock IC has been equipped to ensure that the instrument is traceable via regular calibration. The device will automatically generate warning notifications when the calibration deadline has exceeded.

## Multi-Channel Testing System (Optional)

The TOS9320 high voltage scanner allows for rapid distribution of testing voltage from the main unit to multiple testing points for withstanding voltage and insulation resistance testing. Channels can be controlled via an external device through the rear panel CONTROLLER INTERFACE connector. The scanner can also be used standalone or with an external control device for other Kikusui withstanding voltage and insulation resistance testing instruments. Hipot tests for electronic devices with multiple testing points have never been easier. (See Application P9)

[High-voltage scanner TOS9320]




▲Front panel



▲Rear panel

- Output can be expanded to four channels with one high-voltage scanner. The electric potential of each channel can be arbitrarily set to high, low, or open, and can be tested at any of these four points.
- Up to four high voltage scanners (total 16 channels) can be connected to each unit.
- Output of each channel and contact with testing points can be easily monitored.

[4 channel test system]

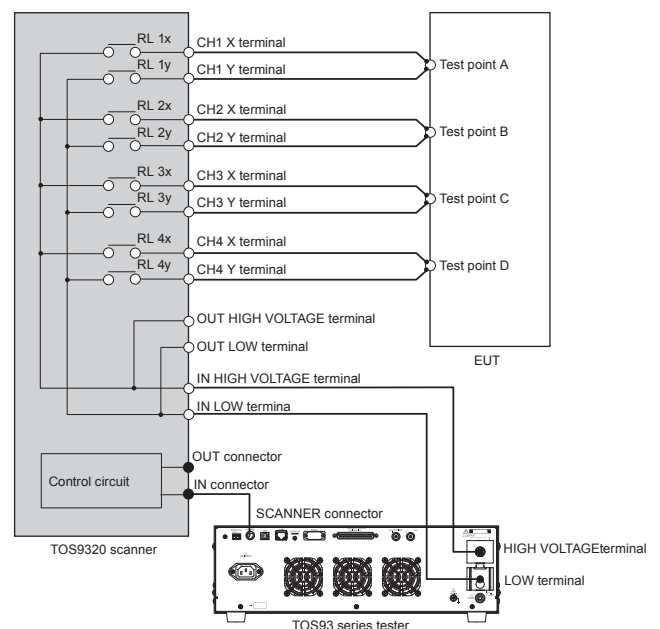




# Application

## Leakage Current Test

Compatible with medical device leakage current testing (patient current)! (TOS9303LC only)

### ●Test Example

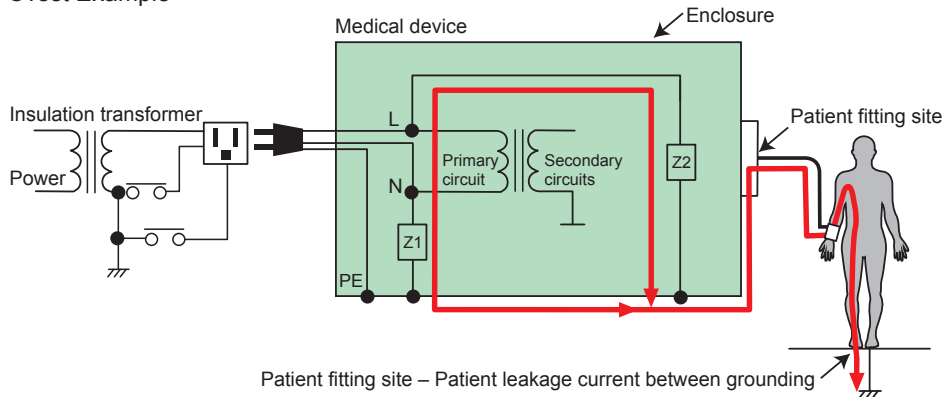

### What is patient leakage current testing?

This test measures current flowing from the point of contact between a medical instrument and a simulated human body network to the ground. If the measurement does not exceed a value deemed harmful to a human being as defined in international safety standards, the product is considered safe and compliant to electric shock prevention requirements.

### Easy Test Condition Programmability


Internal measurement circuit networks (I IEC60601-1) enable easily programmable test conditions.

\*For details on other internally installed measurement circuit networks, see Specifications (P21).



▲TOS9303LC

Setting test conditions

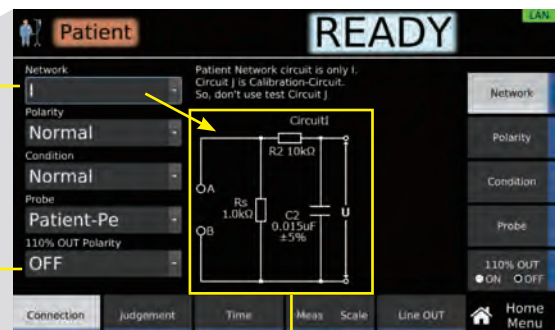

Measurement circuit network (network I IEC60601-1)


## Electrical safety standard testing for automotive components

Compatible with both AC and DC, the TOS9303LC complies with a wide variety of safety tests for EV batteries, automotive charging devices and charging connectors. This "all-in-one" safety analyzer can meet the needs of nearly all automotive electrical safety standards.

*All in One!*

ACW DCW IR EC LC

### IEC61851-21 etc.

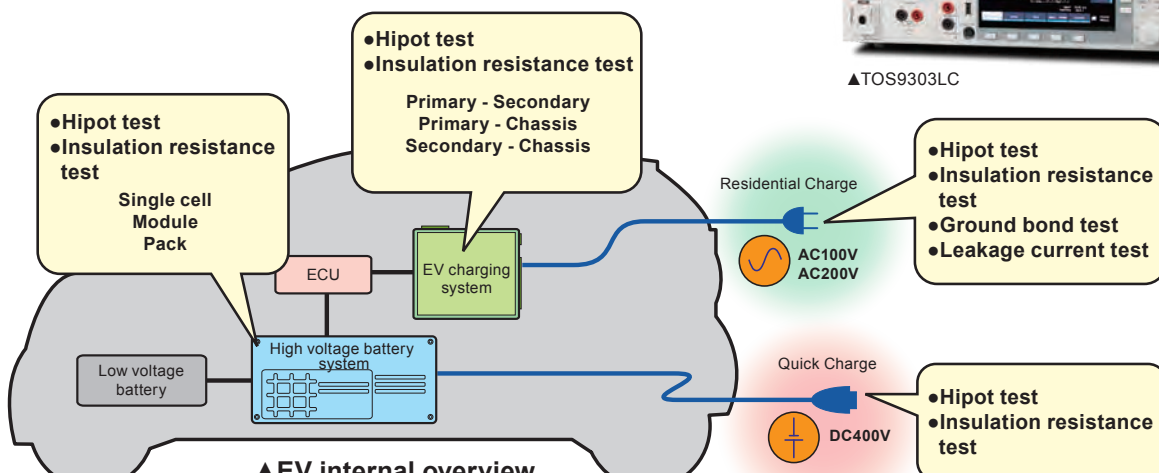




## PV (solar battery) module withstanding voltage/insulation resistance testing

Withstanding voltage tests such as IEC61730-2 and JIS C 8992-2 require testing voltage to be drastically increased (4 times the maximum system voltage + 2000 V) and maintained for 1 minute.

[Voltage 1000 V adaptation grade A example]


$$1000 \text{ V} \times 4\text{-fold} + 2000 \text{ V} = \text{Test voltage : } 6000 \text{ V}$$

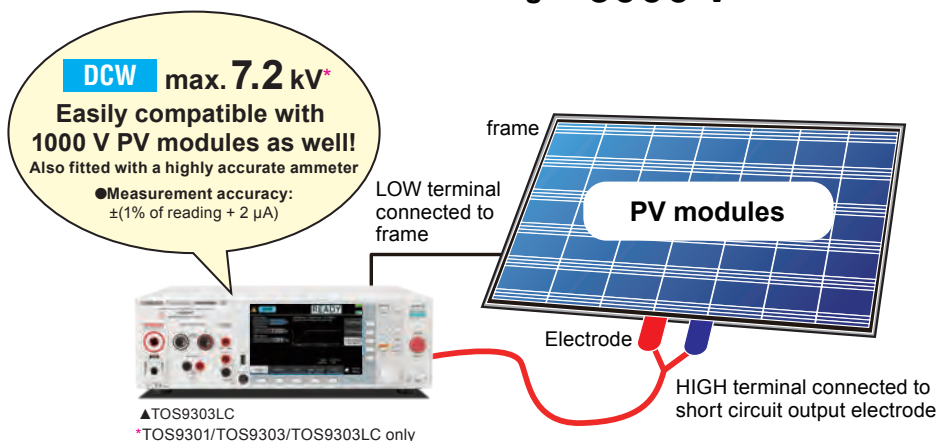

## Partial discharge

[EUT (example): small motors, transformers, insulating materials, etc.]

The partial discharge test detects the state before dielectric breakdown, so it can detect potential defects and manufacturing variations that cannot be detected by the conventional withstand voltage test.

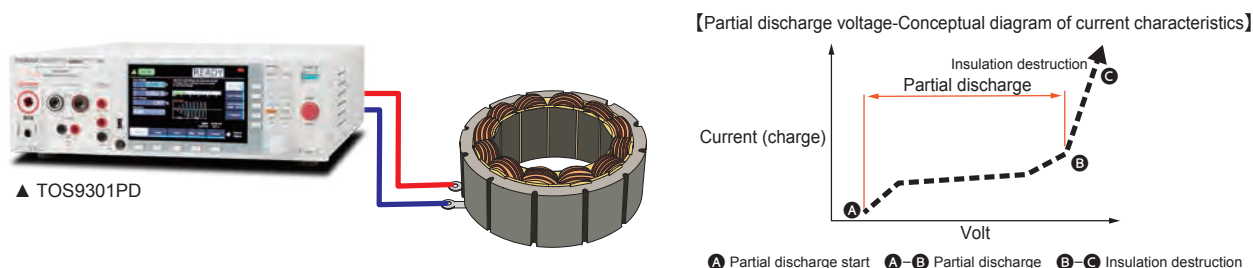


## Multi-channel withstanding voltage/insulation resistance testing

Multiple testing points can be simultaneously tested to cut costs and save time!

The TOS9320 high voltage scanner allows for multi channel expansion for the TOS9300 series as well as previous models.

[16CH Test system]

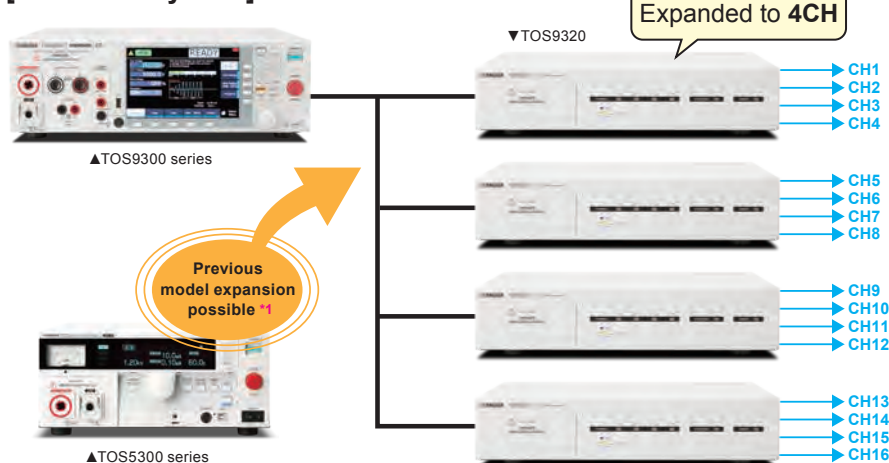

# Exterior Design

## Front panel

### ●TOS9303LC

#### DANGER LED

Lights red when the power is turned on, when a test is in progress, when a high voltage is being output, or when there is residual voltage at the output terminals. On the TOS9303LC, the LED also lights red when supply voltage is being supplied to the EUT.

#### USB connector

Used for external keyboard as well as memory for settings and test results. Also used for import/export of programs and firmware updates.

#### Menu keys

Switch display.

#### Withstanding voltage, insulation resistance

Common for all models.

#### HIGH VOLTAGE terminal

Outputs high test voltage.

#### LOW terminal

Outputs low test voltage (with cable lock).

#### Eath continuity test

Not available for TOS9300 and TOS9301.

#### Leakage current test

TOS9303LC only.

#### Function keys

#### Sub-function keys

#### REMOTE connector

For connection of optional remote control box and test probes.

#### Rotary knob

Select item and enter numbers/characters.

#### START switch

Start test.

#### Numeric keypad

For value input.

#### STOP button

Stops test and clears current status. Returns to Home menu screen.

#### POWER switch

Turn power on/off.

## Rear panel

### ●TOS9303LC

#### SCANNER connector

Connect to optional high voltage scanner.

#### USB port

For remote control.

#### STATUS OUT connector

Connects optional products.

#### LAN port

For remote control.

#### RS232C port

For remote control.

#### SIGNAL I/O connector

I/O signal connector for control via external signals.

#### I terminal

Signal output terminal for monitoring current waveforms for withstanding voltage tests.

#### Withstanding voltage, insulation resistance

Common for all models.

#### V terminal

Signal output terminal for monitoring voltage waveforms for withstanding voltage tests.

#### Leakage current test

TOS9303LC only.

#### HIGH VOLTAGE terminal

Outputs high test voltage.

#### LOW terminal

Outputs low test voltage (with cable lock).

#### DC OUT 5 V terminal

Connects optional products.

#### AC INPUT inlet

100 V to 120 V / 200 V to 240 V

#### Ipd terminal

Signal output terminal for monitoring the discharge waveforms of partial discharge.

#### Qpd terminal

Signal output terminal for monitoring the electric charge waveforms of partial discharge.

### ●TOS9301PD





## Display (Each menu screen)

### ●TOS9303LC screen example

Test mode  
Select test type.

Test status

LAN connection status

Test condition setting

▲Home Menu  
Set conditions for each test. Execute test.

Current menu screen  
Press menu key to switch between menus.

Test mode  
Select test type.

▲Function Menu  
Displays summary of settings for each test. Switch test modes.

▲Program Menu

▲Memory Menu

▲System Menu

# Specifications

Unless specified otherwise, the specifications are for the following settings and conditions.

- The product is warmed up for at least 30 minutes.
- TYP: These are typical values that are representative of situations where the product operates in an environment with an ambient temperature of 23 °C. These values do not guarantee the performance of this product.
- setting: Indicates a setting. • range: Indicates the rated value of each range. • reading: Indicates a readout value.
- The various tests are abbreviated as follows: ACW: AC withstanding voltage, DCW: DC withstanding voltage, IR: insulation resistance, EC: earth continuity, LC: leakage current, TC: touch current, PCC: protective conductor current, Patient: patient leakage current, Meter: meter mode

## ■ Withstanding Voltage Test

### [AC Output function]

Item			TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
AC output section	Output range	Resolution	0.050 kV to 5.000 kV					
		Setting accuracy	1 V					
		±(1.2 % of setting + 0.02 kV) (at no load)						
	Max. rated load *1		500 VA(5 kV / 100 mA)					
	Max. rated current		100 mA (when the output voltage is 0.2 kV or higher)					
	Transformer rating		500 VA					
	Output voltage waveform *2		Sine					
	Distortion	2 % or less. (when the output voltage is 0.5 kV or higher and no load or a pure resistive load is connected)						
		√2 ± 3 % (0.8 V or higher)						
	Frequency		50 Hz / 60 Hz					
	Accuracy	±0.1 %						
		±3 % or less (when changing from maximum rated load to no load)						
Short-circuit current		200 mA or more (output voltage 0.5 kV or higher)						
Output method		PWM switching						
Start voltage			The voltage at the start of the test can be set.					
		Setting range	1 % to 99 % of the test voltage					
		Resolution	1 %					
Output voltage monitor function			If the output voltage exceeds ±(10 % of setting + 0.05 kV), the output is turned off, and the protection function is activated.					

### [DC Output function]

Item			TOS9301	TOS9301PD	TOS9303	TOS9303LC
DC output section	Output voltage range		0.050 kV to 7.200 kV			
		Resolution	1 V			
		Setting accuracy	±(1.2 % of setting + 0.02 kV)			
	Max. rated load *1		100 W (5 kV/20 mA, 7.2 kV/13.9 mA)			
	Max. rated current		20 mA			
	Ripple	7.2 kV no load	20 Vp-p (TYP)			
		Max. rated load	50 Vp-p (TYP)			
	Voltage regulation		1 % or less (when changing from maximum rated load to no load)			
	Short-circuit current		100 mA (TYP) (200 mA peak)			
Discharge function		Forced discharge after test completion (discharge resistance: 125 kΩ)				
Start voltage			The voltage at the start of the test can be set.			
		Setting range	1 % to 99 % of the test voltage			
		Resolution	1 %			
Output voltage monitor function			If the output voltage exceeds ±(10 % of setting + 0.05 kV), the output is turned off, and the protection function is activated.			

- \*1 When tests are performed consecutively, output time limit and rest time may become necessary depending on the upper limit setting
- \*2 If an AC voltage is applied to a capacitive load, the output voltage may rise higher than at no load depending on the load capacitance. Further, waveform distortions may occur if an EUT whose capacitance is dependent on voltage (for example, an EUT that consists of ceramic capacitors) is connected as the load. However, if the test voltage is 1.5 kV, the effect of a capacitance of 1 000 pF or less can be ignored. Because the product's high-voltage power supply uses the PWM switching method, if the test voltage is 500 V or less, the switching and spike noise proportions are large. The lower the test voltage, the greater the waveform is distorted.

### [Measurement function]

Item		TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
Voltmeter	Measurement range	0 kV to 7.5 kV AC/DC					
	Resolution	0.1 V					
	Accuracy	±(1.2 % of reading + 0.005 kV)					
	Response	Can be switched between true rms and mean-value response rms conversion. Peak-value response in a separate system (the peak-value response is for measuring the dielectric breakdown voltage while rising)					
	Hold function	The voltage measurement after a test is finished is held while the pass/fail judgment is displayed.					
Ammeter *1 *2	Measurement range	AC: 0.00 mA to 110 mA, DC: 0.00 mA to 22 mA (Current including the active component and reactive component)					
	Accuracy	±(1 % of reading + 2 µA) (active component)					
	Response	Can be switched between true rms and mean-value response rms conversion.					
	Hold function	The current measurement after a test is finished is held while the pass judgment is displayed.					
	Offset cancel function	Cancels up to 10 mA of the current flowing through the insulation resistance and stray capacitance components across output cables and the like (resistance component only for DC tests). OFF function available.					
	Calibration	Active component: Calibrated with the rms of a sine wave using a pure resistive load. Reactive component: Not calibrated.					

- \*1 During AC voltage tests, current also flows in the stray capacitance of items such as the test leads and tools.  
For details on stray capacitance, see "Stray Capacitance of AC Withstanding Voltage Tests"
- \*2 When the temperature and humidity are high, erroneous current from the product's internal and external high-voltage wiring sections to ground increases. When the humidity exceeds 70 %, an erroneous current of about 50 µA may be generated.



## [Judgment function]

Item			TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC	
Current judgment operation			The output is shut off when a judgment is made. Buzzer volume level can be set in the range of 0 (OFF) to 10 for pass and fail separately. In an auto test, the buzzer is valid only for the judgment that takes place at the end of the program.						
	UPPER FAIL	Judgment method	UPPER FAIL results when a current greater than or equal to the Upper limit is detected. For DCW, judgment is not made during the judgment delay (Judge Delay).						
		Display	"Upper-FAIL" is displayed.						
		Buzzer	On						
	LOWER FAIL	SIGNAL I/O	The Upper-FAIL signal is generated continuously until a STOP signal is received.						
		Judgment method	LOWER FAIL results when a current less than or equal to the Lower limit is detected. Judgment is not made during Voltage rise time or Voltage fall time of an ACW test.						
		Display	"Lower-FAIL" is displayed.						
	PASS	Buzzer	On						
		SIGNAL I/O	The Lower-FAIL signal is generated continuously until a STOP signal is received.						
		Judgment method	PASS judgment is made if Upper-FAIL or Lower-FAIL has not occurred when the test time elapses.						
Display		"PASS" is displayed.							
	dV/dt FAIL	Buzzer	On (fixed to 50 ms)						
		SIGNAL I/O	The PASS signal is generated for the length of time specified by the Pass Hold set-ting. If Pass Hold is set to Infinity, the PASS signal is generated continuously until a STOP signal is received.						
		Judgment method	Monitors the voltage rise rate during Voltage rise time. This is valid when Auto setting of the judgment delay (Delay Auto) is set to on and the output voltage is 200 V or more. The output is shut off when a judgment is made. Buzzer volume level can be set in the range of 0 (OFF) to 10 for pass and fail separately.						
		Upper limit setting range	Display	" Upper-FAIL(dv/dt)" is displayed.					
			Buzzer	ON					
			SIGNAL I/O	The U FAIL signal is generated continuously until a STOP signal is received.					
	Lower limit setting range			AC: 0.01 mA to 110.00 mA, DC: 0.01 mA to 21.00 mA					
	Judgment accuracy *1 *2			±(1 % of setting + 5 μA)					
	Current detection method			Compares to the reference value using the following method. Calculate true rms values, convert mean-value responses to rms values					
Response speed (filter) switching			Switches the current detection response speed (sensitivity) used in UPPER FAIL judgment between five levels in ACW and DCW tests.						

\*1 During AC voltage tests, current also flows in the stray capacitance of items such as the test leads and tools. For details on stray capacitance, see "Stray Capacitance of AC Withstanding Voltage Tests"

\*2 When the temperature and humidity are high, erroneous current from the product's internal and external high-voltage wiring sections to ground increases. When the humidity exceeds 70 %, an erroneous current of about 50 µA may be generated.

## [Timer function]

Item	TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
Voltage rise time settings range	0.1 s to 200.0 s					
Voltage fall time setting time *1	0.1 s to 200.0 s, OFF					
Test time setting range	0.1 s to 1000.0 s, OFF					
Judgment delay (Judge Delay) setting range *2	0.1 s to 100.0 s, AUTO *3 (DCW only)					
Accuracy	±(100 ppm of setting + 20 ms) (excluding the fall time)					

\*1 This setting is used only when a PASS judgment occurs in ACW and DCW tests. During a DCW test, the voltage may not drop all the way within the set time because of the electrostatic capacity inside the product and the EUT.

\*2 Less than the sum of the rise time and fall time.

\*3 If Delay Auto is set to on, LOWER judgment is not made until the charge time ends.

## [Other specifications]

Item	TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
Analog monitor *1	Outputs a voltage signal according to the current waveform or voltage waveform					
Grounding mode (GND)	I	Current waveform: Scale 50 mA/1 V				
	V	Voltage waveform: Scale 1 kV/1 V				
	Low	Can be switched between Low and Guard.				
	Guard *2	GND is connected to the low terminal. Measures the current flowing across the low terminal and chassis (normal applications).				
	Guard *2	GND is connected to Guard. Measures only the current flowing through the low terminal (current flowing through the chassis is not measured) (high sensitivity, high accuracy measurement applications).				

\*1 Monitor signal output is isolated from the chassis (earth). If you connect an oscilloscope or an external device whose BNC shield is grounded, be sure to set the grounding mode (GND) to Guard. The value is not calibrated.

\*2 If there is a possibility that the EUT or tools and the like will be grounded or if you are uncertain, do not set GND to Guard. Doing so is extremely dangerous because the ammeter will be shorted and will not be able to measure current. For normal applications, set GND to Low.

# Specifications

## ■ Insulation Resistance Test

[Output function]

Item			TOS9300	TOS9301	TOS9301PD	TOS9303	TOS9303LC
Negative polarity	Output voltage range		-0.025 kV to -1 kV				
		Resolution	1 V				
		Setting accuracy	±(1.2 % of setting + 0.002 kV)				
	Max. rated load		1 W (-1 kV/1 mA)				
	Ripple	1 kV no load	2 Vp-p or less				
		Max. rated load	10 Vp-p or less				
Short-circuit current			12 mA or less				
Positive polarity *1	Output voltage range		-	+0.05 kV to +7.2 kV			
		Resolution		1 V			
		Setting accuracy		±(1.2 % of setting + 0.02 kV)			
	Max. rated load			7.2 W(7.2 kV/1 mA)			
	Ripple	1 kV no load		20 Vp-p or less			
		Max. rated load		50 Vp-p or less			
Short-circuit current			100 mA (TYP) (200 mA peak)				
Max. rated current			1 mA				
Voltage regulation			1 % or less (when changing from maximum rated load to no load)				
Discharge function			Forced discharge after test completion (discharge resistance: 20 kΩ)				
Output voltage monitor function			If the output voltage exceeds ±(10 % of setting + 0.05 kV), the output is turned off, and the protection function is activated.				

\*1 TOS9300 are not supported.

[Measurement function]

Item			TOS9300	TOS9301	TOS9301PD	TOS9303	TOS9303LC
Voltmeter	Measurement range		Negative polarity: 0 Vdc to -1200 Vdc, positive polarity: 0 Vdc to 7500 Vdc				
	Resolution		0.1 V				
	Accuracy		Negative polarity: ±(1 % of reading + 1 V), positive polarity: ±(1.2 % of reading + 1 V)				
Resistance meter	Measurement range		0.001 MΩ to 100.0 GΩ (in the range of maximum rated current of 1 mA to 5 nA)				
	Accuracy *1 *2 (when GND is set to Guard) (i: measured current)(R: measurement resistance)	5 nA ≤ i ≤ 50 nA *3	500.000 MΩ ≤ R < 1.000 GΩ:		±(15 % of reading + 0.5 MΩ)		
			1.000 GΩ ≤ R < 10.000 GΩ:		±(15 % of reading + 5 MΩ)		
			10.000 GΩ ≤ R ≤ 100.000 GΩ:		±(20 % of reading + 200 MΩ)		
		50 nA < i ≤ 100 nA *3	200.000 MΩ ≤ R < 1.000 GΩ:		±(10 % of reading + 0.5 MΩ)		
			1.000 GΩ ≤ R < 10.000 GΩ:		±(10 % of reading + 5 MΩ)		
			10.000 GΩ ≤ R < 50.000 GΩ:		±(10 % of reading + 50 MΩ)		
		100 nA < i ≤ 200 nA *4	50.000 GΩ ≤ R ≤ 100.000 GΩ:		±(20 % of reading + 200 MΩ)		
			100.000 MΩ ≤ R < 1.000 GΩ:		±(7 % of reading + 0.5 MΩ)		
			1.000 GΩ ≤ R < 2.000 GΩ:		±(7 % of reading + 5 MΩ)		
		200 nA < i ≤ 1 μA *4	2.000 GΩ ≤ R < 10.000 GΩ:		±(7 % of reading + 10 MΩ)		
			10.000 GΩ ≤ R < 50.000 GΩ:		±(7 % of reading + 100 MΩ)		
			10.000 MΩ ≤ R < 100.000 MΩ:		±(5 % of reading + 0.05 MΩ)		
	Accuracy *5 (when GND is set to Low) (i: measured current)(R: measurement resistance)	1 μA < i ≤ 1 mA *4	100.000 MΩ ≤ R < 1.000 GΩ:		±(5 % of reading + 0.5 MΩ)		
			1.000 GΩ ≤ R < 10.000 GΩ:		±(5 % of reading + 5 MΩ)		
			10.000 GΩ ≤ R < 25.000 GΩ:		±(5 % of reading + 50 MΩ)		
		5 nA ≤ i ≤ 50 nA *3	0.001 MΩ ≤ R < 10.000 MΩ:		±(2 % of reading + 0.003 MΩ)		
			10.000 MΩ ≤ R < 100.000 MΩ:		±(2 % of reading + 0.03 MΩ)		
			100.000 MΩ ≤ R < 1.000 GΩ:		±(2 % of reading + 0.3 MΩ)		
		50 nA < i ≤ 100 nA *3	1.000 GΩ ≤ R < 5.000 GΩ:		±(2 % of reading + 3 MΩ)		
			500.000 MΩ ≤ R < 1.000 GΩ:		±(25 % of reading + 0.5 MΩ)		
			1.000 GΩ ≤ R < 10.000 GΩ:		±(25 % of reading + 5 MΩ)		
		100 nA < i ≤ 200 nA *4	10.000 GΩ ≤ R ≤ 100.000 GΩ:		±(30 % of reading + 200 MΩ)		
			200.000 MΩ ≤ R < 1.000 GΩ:		±(20 % of reading + 0.5 MΩ)		
			1.000 GΩ ≤ R < 10.000 GΩ:		±(20 % of reading + 5 MΩ)		
	200 nA < i ≤ 1 μA *4	10.000 GΩ ≤ R < 50.000 GΩ:		±(20 % of reading + 50 MΩ)			
		50.000 GΩ ≤ R ≤ 100.000 GΩ:		±(30 % of reading + 200 MΩ)			
		100.000 MΩ ≤ R < 1.000 GΩ:		±(10 % of reading + 0.5 MΩ)			
	1 μA < i ≤ 1 mA *3	1.000 GΩ ≤ R < 2.000 GΩ:		±(10 % of reading + 5 MΩ)			
		2.000 GΩ ≤ R < 10.000 GΩ:		±(10 % of reading + 10 MΩ)			
		10.000 GΩ ≤ R < 50.000 GΩ:		±(10 % of reading + 100 MΩ)			
	5 nA ≤ i ≤ 50 nA *3	10.000 MΩ ≤ R < 100.000 MΩ:		±(5 % of reading + 0.05 MΩ)			
		100.000 MΩ ≤ R < 1.000 GΩ:		±(5 % of reading + 0.5 MΩ)			
		1.000 GΩ ≤ R < 10.000 GΩ:		±(5 % of reading + 5 MΩ)			
	50 nA < i ≤ 100 nA *3	10.000 GΩ ≤ R < 25.000 GΩ:		±(5 % of reading + 50 MΩ)			
		0.001 MΩ ≤ R < 10.000 MΩ:		±(2 % of reading + 0.003 MΩ)			
		10.000 MΩ ≤ R < 100.000 MΩ:		±(2 % of reading + 0.03 MΩ)			
	100 nA < i ≤ 200 nA *4	100.000 MΩ ≤ R < 1.000 GΩ:		±(2 % of reading + 0.3 MΩ)			
		1.000 GΩ ≤ R < 5.000 GΩ:		±(2 % of reading + 3 MΩ)			
Hold function			The resistance measurement after a test is finished is held while the pass judgment is displayed.				
Offset cancel function			Cancels up to 2000 GΩ of the unnecessary insulation resistance across output cables and the like. OFF function available.				

\*1 Humidity: 70 %rh or less (no condensation), when there is no interference caused by wobbly test leads or other problems.

\*2 If the grounding mode (GND) is set to low in a highly humid environment, leakage current to ground will be generated from the high-voltage wiring sections inside the product and the high-voltage wiring sections between the product and the EUT. This leakage current ranges from several nA to several tens of nA depending on the usage and wiring conditions of the optional TOS9320 high voltage scanner and greatly affects measurement accuracy. The effects of leakage current can be reduced by making measurements with the offset enabled.

\*3 Add 10 % to the accuracy when measuring 100 V or less.

\*4 Add 5 % to the accuracy when measuring 100 V or less.



## [Judgment function]

Item		TOS9300	TOS9301	TOS9301PD	TOS9303	TOS9303LC
Behavior based on judgment		The output is shut off when a judgment is made. Buzzer volume level can be set in the range of 0 (OFF) to 10 for pass and fail separately. In an auto test, the buzzer is valid only for the judgment that takes place at the end of the program.				
UPPER FAIL	Judgment method	UPPER FAIL results when a resistance greater than or equal to the Upper limit is detected. Judgment is not made during or Voltage rise time.				
	Display	"Upper-FAIL" is displayed.				
	Buzzer	On				
	SIGNAL I/O	The Upper-FAIL signal is generated continuously until a STOP signal is received.				
LOWER FAIL	Judgment method	LOWER FAIL results when a resistance less than or equal to the Lower limit is detected. Judgment is not made during the judgment delay (Judge Delay).				
	Display	"Lower-FAIL" is displayed.				
	Buzzer	On				
	SIGNAL I/O	The Lower-FAIL signal is generated continuously until a STOP signal is received.				
PASS	Judgment method	PASS judgment is made if Upper-FAIL or Lower-FAIL has not occurred when the test time elapses.				
	Display	"PASS" is displayed.				
	Buzzer	On (fixed to 50 ms)				
	SIGNAL I/O	The PASS signal is generated for the length of time specified by the Pass Hold setting. If Pass Hold is set to Infinity, the PASS signal is generated continuously until a STOP signal is received.				
Voltage rise rate judgment operation		Monitors the voltage rise rate during Voltage rise time. This is valid when Auto setting of the judgment delay (Delay Auto) is set to on and the output voltage is 200 V or more. The output is shut off when a judgment is made. Buzzer volume level can be set in the range of 0 (OFF) to 10 for pass and fail separately.				
dV/dt FAIL	Judgment method	When the voltage rise rate (dV/dt) is less than 1 V/s.				
	Display	" Lower-FAIL(dv/dt)" is displayed.				
	Buzzer	On				
	SIGNAL I/O	The L FAIL signals are generated continuously until a STOP signal is received.				
Upper limit setting range		0.001 MΩ to 100.000 GΩ (in the range up to the maximum rated current), OFF				
Lower limit setting range		0.000 MΩ to 99.999 GΩ (in the range up to the maximum rated current), OFF. Setting 0.000 is equivalent to OFF.				
Accuracy *1 *2 *3 (when GND is set to Guard) (i: measured current) (R: measurement resistance)	5 nA ≤ i ≤ 50 nA *4	500.000 MΩ ≤ R < 1.000 GΩ: ±(15 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(15 % of setting + 15 MΩ)				
		10.000 GΩ ≤ R ≤ 100.000 GΩ: ±(20 % of setting + 210 MΩ)				
	50 nA < i ≤ 100 nA *4	200.000 MΩ ≤ R < 1.000 GΩ: ±(10 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(10 % of setting + 15 MΩ)				
		10.000 GΩ ≤ R < 50.000 GΩ: ±(10 % of setting + 60 MΩ)				
	100 nA < i ≤ 200 nA *5	50.000 GΩ ≤ R ≤ 100.000 GΩ: ±(20 % of setting + 210 MΩ)				
		100.000 MΩ ≤ R < 1.000 GΩ: ±(7 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 2.000 GΩ: ±(7 % of setting + 15 MΩ)				
	200 nA < i ≤ 1 μA *5	2.000 GΩ ≤ R < 10.000 GΩ: ±(7 % of setting + 20 MΩ)				
		10.000 GΩ ≤ R < 50.000 GΩ: ±(7 % of setting + 110 MΩ)				
		10.000 MΩ ≤ R < 100.000 MΩ: ±(5 % of setting + 0.06 MΩ)				
	1 μA < i ≤ 1 mA *5	100.000 MΩ ≤ R < 1.000 GΩ: ±(5 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(5 % of setting + 15 MΩ)				
		10.000 GΩ ≤ R < 25.000 GΩ: ±(5 % of setting + 60 MΩ)				
Accuracy *6 (when GND is set to Low) (i: measured current) (R: measurement resistance)	5 nA ≤ i ≤ 50 nA *4	0.001 MΩ ≤ R < 10.000 MΩ: ±(2 % of setting + 0.013 MΩ)				
		10.000 MΩ ≤ R < 100.000 MΩ: ±(2 % of setting + 0.04 MΩ)				
		100.000 MΩ ≤ R < 1.000 GΩ: ±(2 % of setting + 0.31 MΩ)				
	50 nA < i ≤ 100 nA *4	1.000 GΩ ≤ R < 5.000 GΩ: ±(2 % of setting + 13 MΩ)				
		500.000 MΩ ≤ R < 1.000 GΩ: ±(25 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(25 % of setting + 15 MΩ)				
	100 nA < i ≤ 200 nA *5	10.000 GΩ ≤ R ≤ 100.000 GΩ: ±(30 % of setting + 210 MΩ)				
		200.000 MΩ ≤ R < 1.000 GΩ: ±(20 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(20 % of setting + 15 MΩ)				
	200 nA < i ≤ 1 μA *5	10.000 GΩ ≤ R < 50.000 GΩ: ±(20 % of setting + 60 MΩ)				
		50.000 GΩ ≤ R ≤ 100.000 GΩ: ±(30 % of setting + 210 MΩ)				
		100.000 MΩ ≤ R < 1.000 GΩ: ±(10 % of setting + 0.51 MΩ)				
	1 μA < i ≤ 1 mA *5	1.000 GΩ ≤ R < 2.000 GΩ: ±(10 % of setting + 15 MΩ)				
		2.000 GΩ ≤ R < 10.000 GΩ: ±(10 % of setting + 20 MΩ)				
		10.000 GΩ ≤ R < 50.000 GΩ: ±(10 % of setting + 110 MΩ)				
	5 nA ≤ i ≤ 50 nA *4	10.000 MΩ ≤ R < 100.000 MΩ: ±(5 % of setting + 0.06 MΩ)				
		100.000 MΩ ≤ R < 1.000 GΩ: ±(5 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(5 % of setting + 15 MΩ)				
	50 nA < i ≤ 100 nA *4	10.000 GΩ ≤ R < 25.000 GΩ: ±(5 % of setting + 60 MΩ)				
		0.001 MΩ ≤ R < 10.000 MΩ: ±(2 % of setting + 0.013 MΩ)				
		10.000 MΩ ≤ R < 100.000 MΩ: ±(2 % of setting + 0.04 MΩ)				
		100.000 MΩ ≤ R < 1.000 GΩ: ±(2 % of setting + 0.31 MΩ)				
	100 nA < i ≤ 200 nA *5	1.000 GΩ ≤ R < 5.000 GΩ: ±(2 % of setting + 13 MΩ)				
		500.000 MΩ ≤ R < 1.000 GΩ: ±(25 % of setting + 0.51 MΩ)				
		1.000 GΩ ≤ R < 10.000 GΩ: ±(25 % of setting + 15 MΩ)				

\*1 Making judgments on 200 μA or less requires at least 3 seconds after the rise time ends. Making judgments when the low pass filter is set to on requires at least 10 seconds after the rise time ends.

\*2 Humidity: 70 %rh or less (no condensation), when there is no interference caused by wobbly test leads or other problems.

\*3 If the grounding mode (GND) is set to low in a highly humid environment, leakage current to ground will be generated from the high-voltage wiring sections inside the product and the high-voltage wiring sections between the product and the EUT. This leakage current ranges from several nA to several tens of nA depending on the usage and wiring conditions of the optional TOS9320 high voltage scanner and greatly affects measurement accuracy. The effects of leakage current can be reduced by making measurements with the offset enabled.

\*4 Add 10 % to the accuracy when measuring 100 V or less.

\*5 Add 5 % to the accuracy when measuring 100 V or less.

\*6 When the measured current is limited to 100 nA or more (no condensation) when the humidity is 50 %rh or less, no external disturbance is present such as swinging test leads, and the effect is enabled.

# Specifications

## [Timer function]

Item	TOS9300	TOS9301	TOS9301PD	TOS9303	TOS9303LC
Voltage rise time settings range	0.1 s to 200.0 s				
Test time setting range	0.1 s to 1000.0 s, OFF				
Judgment delay (Judge Delay) setting range *1	0.1 s to 100.0 s, AUTO *2				
Accuracy *3	±(100 ppm of setting + 20 ms)				

\*1 Less than the sum of the rise time and fall time.

\*2 If Delay Auto is set to on, UPPER judgment is not made until the charge time ends.

\*3 This excludes fall time.

## [Other specifications]

Item		TOS9300	TOS9301	TOS9301PD	TOS9303	TOS9303LC
Grounding mode (GND)		Can be switched between Low and Guard.				
	Low	GND is connected to the low terminal. Measures the current flowing across the low terminal and chassis (normal applications).				
	Guard *1	GND is connected to Guard. Measures only the current flowing through the low terminal (current flowing through the chassis is not measured) (high sensitivity, high accuracy measurement applications).				
Filter function		A low-pass filter can be inserted into the ammeter measurement circuit. *2				

\*1 If there is a possibility that the EUT or tools and the like will be grounded or if you are uncertain, do not set GND to Guard. Doing so is extremely dangerous because the ammeter will be shorted and will not be able to measure current. For normal applications, set GND to Low.

\*2 When the low pass filter is on, a judgment delay of at least 5 seconds and a test time are required.

## ■ Earth Continuity Test

### [Output function]

Item		TOS9302	TOS9303	TOS9303LC
		3.0 A to 42.0 A AC/DC		
Current setting range *1	Resolution	0.1 A		
	Accuracy	±(1 % of setting + 0.4 A)		
AC	Maximum rated output *2	220 VA (at the output terminal)		
	Distortion	2 % or less (20 A or more, using a 0.1 Ω pure resistive load)		
	Frequency	Select 50 Hz or 60 Hz. Sine		
	Accuracy	±200 ppm		
	Open terminal voltage	6 Vrms or less		
	Output method	PWM switching		
DC	Maximum rated output	220 W (at the output terminal)		
	Ripple	±0.4 Ap-p or less (TYP)		
	Open terminal voltage	6.0 V or less		

\*1 No greater than the maximum rated output and resistance no greater than the output terminal voltage 5.4 V.

\*2 When tests are performed consecutively, output time limit and rest time may become necessary depending on the upper limit setting.

### [Measurement function]

Item		TOS9302	TOS9303	TOS9303LC
Output ammeter	Measurement range	0.0 A to 45.0 A AC/DC		
	Resolution	0.01 A		
	Accuracy	±(1 % of reading + 0.2 A)		
	Response	AC: true rms value; DC: mean value		
	Hold function	The current measurement after a test is finished is held while the pass or fail judgment is displayed.		
Output voltmeter	Measurement range	AC: 0.00 V to 6.00 V, DC: 0.00 V to 8.50 V		
	Resolution	0.001 V		
	Offset cancel function	Cancels up to 5 V (AC/DC) of the unnecessary voltage from measurements. OFF function available.		
	Accuracy	±(1 % of setting + 0.02 V)		
	Response	AC: true rms value; DC: mean value		
Resistance meter	Hold function	The voltage measurement after a test is finished is held while the pass or fail judgment is displayed.		
	Measurement range *1	1 mΩ to 600 mΩ		
	Resolution	1 mΩ		
	Offset cancel function	Cancels up to 10 Ω of the unnecessary resistance from measurements. OFF function available.		
	Accuracy	±(2 % of reading + 3 mΩ)		
	Hold function	The resistance measurement after a test is finished is held while the pass judgment is displayed.		

\*1 Calculated from the measured output voltage and measured output current.

### [Judgment function]

Item			TOS9302	TOS9303	TOS9303LC
Behavior based on judgment	UPPER FAIL	Judgment method	Judgment based on resistance or sensing voltage can be selected. The output is shut off when a judgment is made. Buzzer volume level can be set in the range of 0 (OFF) to 10 for pass and fail separately. In an auto test, the buzzer is valid only for the judgment that takes place at the end of the program.		
		Display	UPPER FAIL results when a resistance greater than or equal to the Upper limit is detected or when a sensing voltage is detected. Judgment is not made during a contact check.		
		Buzzer	"U-FAIL" is displayed.		
		SIGNAL I/O	On		
	LOWER FAIL	Judgment method	The U-FAIL signal is generated continuously until a STOP signal is received.		
		Display	LOWER FAIL results when a resistance less than or equal to the lower limit (Lower) is detected or when a sensing voltage is detected.		
		Buzzer	"L-FAIL" is displayed.		
		SIGNAL I/O	On		
	PASS	Judgment method	The L-FAIL signal is generated continuously until a STOP signal is received.		
		Display	PASS judgment is made if U-FAIL or L-FAIL has not occurred when the test time elapses.		
		Buzzer	"PASS" is displayed.		
		SIGNAL I/O	On (fixed to 50 ms)		
Resistance judgment	Upper limit setting range		The PASS signal is generated for the length of time specified by the Pass Hold setting. If Pass Hold is set to Infinity, the PASS signal is generated continuously until a STOP signal is received.		
	Lower limit setting range		0.0001 Ω to 10.0000 Ω		
	Judgment accuracy		0.0000 Ω to 9.9999 Ω		
Voltage judgment	Upper limit setting range		±(2 % of setting + 3 mΩ)		
	Lower limit setting range		0.001 V to 5.000 V AC/DC		
	Judgment accuracy		0.000 V to 4.999 V AC/DC		
Calibration			±(2 % of setting + 0.05 V)		
Contact check function			Calibrated using a pure resistive load (with the rms of a sine wave for AC) Checks that current flows through the test leads and then starts the test. (OFF setting available)		

### [Timer function]

Item		TOS9302	TOS9303	TOS9303LC
Current rise time settings range		0.1 s to 200.0 s		
Current fall time setting time *1		0.1 s to 200.0 s, OFF		
Test time		0.1 s to 1000.0 s, OFF		
Accuracy		±(100 ppm of setting + 20 ms) (excluding the fall time)		

\*1 This setting is used only when a PASS judgment occurs. During a DC test, the voltage may not drop all the way within the set time because of the electrostatic capacity inside the



# Specifications

## ■ Partial Discharge Test

### [Output function]

Item			TOS9301PD
AC output section	Output range	Resolution	0.050 kV to 5.000 kV
		Setting accuracy	1 V
			±(1.2% of setting + 0.02kV) (at no load)
	Max. rated load		250 VA (5 kV/ 50mA)
	Max. rated current		50 mA (when the output voltage is 0.2 kV or higher)
	Output voltage waveform*1		Sine
	Distortion		2 % or less. (when the output voltage is 0.5 kV or higher and no load or a pure resistive load is connected)
			√2 ± 3 % (0.8 V or higher)
	Crest factor		√2 ± 3 % (0.8 V or higher)
	Frequency		50 Hz/60 Hz
		Accuracy	±0.1 %
Voltage regulation		±3 % or less (when changing from maximum rated load to no load)	
Output method		PWM switching	
Output voltage monitor function			If the output voltage exceeds ±(10 % of setting + 0.05 kV), the output is turned off, and the protection function is activated.

\*1 If an AC voltage is applied to a capacitive load, the output voltage may rise higher than at no load depending on the load capacitance. Further, waveform distortions may occur if an EUT whose capacitance is dependent on voltage (for example, an EUT that consists of ceramic capacitors) is connected as the load. However, if the test voltage is 1.5kV, the effect of a capacitance of 1 000pF or less can be ignored. Because the product's high-voltage power supply uses the PWM switching method, if the test voltage is 500 V or less, the switching and spike noise proportions are large. The lower the test voltage, the greater the waveform is distorted.

### [Measurement function]

Item			TOS9301PD
Voltmeter	Measurement range		0.00 kV to 7.50 kV AC/DC
	Resolution		0.1 V
	Accuracy		±(1.2 % of reading + 0.05 kV)
	Response		Can be switched between true rms and peak-value response.
	Hold function		The voltage measurement after a test is finished is held while the pass/fail judgment is displayed.
Electric charge measurement	Electric charge measurement method		IEC60664-1 Edition 3.0 compliant
	Measurement range		0 pC to 10000 pC
	Measurement resolution	100pC range	0.1 pC
		1000pC range	0.1 pC
		10000pC rang	1 pC
	Accuracy*1	100pC range	±(5 % of full scale + 7 pC)
		1000pC range	±(5 % of full scale)
		10000pC rang	±(5 % of full scale)
	Measurement interval		Determined based on the measured values in each cycle of an applied voltage.
	Hold function		The electric charge after a test is finished is held while the pass judgment is displayed.
	Maximum electrostatic capacity of the EUT		10 nF
	Peak hold function		Holds the maximum value during a measurement.
	Filter function		A low-pass filter can be inserted into the electric charge measurement circuit.
	Discharge inception voltage, discharge inception voltage measurement		Measures the voltage at which discharge exceeding a preset electric charge starts and the voltage at which discharge ceases (complies with IEC60664-1 third edition).
	Calibration (Precalibration)		Calibrate using the built-in calibration capacitor (1000 pF).
	Pulse counting function	Counts the number of pulses that have passed through the high-pass filter and makes a FAIL judgment if the count exceeds the upper limit.	
		Upper limit setting range	1 to 100000
	BPF characteristics switching function		Can switch the characteristics of the band-pass filter in the electric charge measuring circuit
			Center frequency
Coupling capacitor			0.01 μF

\*1 When Band Pass Filter is set to 160 kHz.

## [Judgment function]

Item		TOS9301PD
Electric discharge judgment		The output is shut off when a judgment is made.
UPPER FAIL (Current)	Judgment method	A current higher than or equal to the upper limit is measured.
	Display	"Upper-FAIL (Current)" is displayed.
	Buzzer	On
	SIGNAL I/O	The Upper-FAIL signal is generated continuously until a STOP signal is received.
UPPER FAIL (Coulomb)	Judgment method	An electric charge greater than or equal to the upper limit is measured.
	Display	"Upper-FAIL (Coulomb)" is displayed.
	Buzzer	On
	SIGNAL I/O	The Upper-FAIL signal is generated continuously until a STOP signal is received.
UPPER FAIL (Pulse)	Judgment method	A discharge pulse count greater than or equal to the upper limit is measured.
	Display	"Upper-FAIL (Pulse)" is displayed.
	Buzzer	On
	SIGNAL I/O	The Upper-FAIL signal is generated continuously until a STOP signal is received.
PASS	Judgment method	Upper-FAIL does not happen after the test time has elapsed.
	Display	"PASS" is displayed.
	Buzzer	On
	SIGNAL I/O	The PASS signal is generated for the length of time specified by the Pass Hold setting. If Pass Hold is set to Infinity, the PASS signal is generated continuously until a STOP signal is received.
Upper current limit		50 mA (with no calibration)
Upper limit of electric charge (Upper Coulomb)	Setting range	1 pC to 10000 pC
	Accuracy	As per the accuracy of electric charge measurement
Pulse count judgment criteria (Upper Pulse Count) setting range		1 to 100000 (with no calibration)

## [Timer function]

Item		TOS9301PD
Voltage rise time (Rise Time) setting range		0.1 s to 200.0 s
Voltage fall time (Fall Time) setting range *1		0.1 s to 200.0 s, OFF
Test time setting range		0.1 s to 1000.0 s, OFF
Accuracy		±(100 ppm of setting + 20 ms) (excluding Fall Time)

\*1 This setting is used only when PASS judgment occurs.

## [Other specifications]

Item		TOS9301PD
Analog monitor*1		Outputs a voltage signal according to the current waveform, voltage waveform, or electric discharge waveforms.
	V	Voltage waveform: Scale 1kV/1V
	Qpd	Electric discharge: Full scale of the scale measurement range/10 V
	Ipd*2	Partial discharge current waveform

\*1 Monitor signal output is isolated from the chassis (earth).

\*2 The Ipd waveforms are the ones that can be obtained after the actual discharge waveforms have passed the TOS9301PD measurement filter. Therefore, the scale varies according to the frequency response of the discharge waveform.

# Specifications

## ■ Leakage Current Test

### [Measurement function]

Item			TOS9303LC	
Measurement Item	TC			Touch current measurement
		Measurement mode		Uses a measurement circuit network representing the impedance of a human body and measures the voltage drop across a reference resistance to calculate the touch current.
		Probe settings	Enc - Pe	A terminal: measurement terminal (for connecting to the enclosure of the EUT) B terminal: open
			Enc - Enc	A and B terminals: measurement terminal (for connecting to the enclosure of the EUT)
			Enc - Liv	A terminal: measurement terminal (for connecting to the enclosure of the EUT)
	Enc - Neu		B terminal: open	
	PCC			Protective conductor current measurement
		Measurement method		Measures the voltage drop across a reference resistance inserted in the middle of the protective ground line to calculate the protective conductor current. The measurement impedance is 150 Ω.
	Patient			Patient leakage current measurement
		Measurement method		Uses a network conforming to IEC 60601 and measures the voltage drop across a reference resistance to calculate the patient leakage current.
Meter			Measures the current flowing or voltage applied across the A and B terminals (simultaneous measurement not possible).	
	Measurement method	Current measurement	Uses a measurement circuit network representing the impedance of a human body and measures the voltage drop across a refer-ence resistance to calculate the current flowing across the A and B terminals.	
		Voltage measurement	Measures the voltage applied across the A and B terminals.	
		DC		Eliminates AC components and measures only the DC component.
		RMS		Measures the true rms value (switch AC and AC+DC)
		Peak *1	Measures waveform peak values	

\*1 Current measurements may not be stable due to the effects of the power supply line waveform or the wiring environment between the product and the EUT.


### [Measurement circuit network]

Item		TOS9303LC
Network	A (IEC 60990 compliant) *1	(1.5 kΩ // 0.22 μF) + 500 Ω, reference measurement element: 500 Ω
	B (IEC 60990 compliant)	(1.5 kΩ // 0.22 μF) + 500 Ω // (10 kΩ + 22 nF), reference measurement element: 500 Ω, voltage measurement U1 and U3 switchable
	C (IEC 60990 compliant)	(1.5 kΩ // 0.22 μF) + 500 Ω // (10 kΩ + (20 kΩ + 6.2 nF) // 9.1 nF), reference measurement element: 500 Ω, voltage measurement U1 and U3 switchable
	D (Electrical Appliances and Materials Safety Act, etc.)	1 kΩ, reference measurement element: 1 kΩ
	E (Electrical Appliances and Materials Safety Act)	1 kΩ // (10 kΩ + 11.225 nF + 579 Ω), reference measurement element:1 kΩ
	F (UL and the like)	1.5 kΩ // 0.15 μF, reference measurement element: 1.5 kΩ
	G	2 kΩ, reference measurement element: 2 kΩ
	H (IEC 61010-1)	375 Ω // 0.22 μF + 500 Ω, reference measurement element: 500 Ω
	I (Patient, IEC60601-1wet)	1 kΩ // 10 kΩ + 0.015 μF, reference measurement element: 1 kΩ
	J (through)	For voltmeter calibration
	PCC-1	150 Ω, reference measurement element: 150 Ω
	PCC-2 (IEC 60598-1)	150 Ω // 1.5 μF, reference measurement element: 150 Ω
Network constant tolerance		Resistance: ±0.1 %, capacitor 0.15 μF: ±2 %, others: ±1 %
Network accuracy	A, B, C, H	Input voltage vs. output voltage ratio: logical value ± 5 %(according to IEC 60990 Annex L and F)
	E	Input voltage vs. output voltage ratio: logical value ± 5 %
	D, G	Reference measurement element (resistance) ± 1 %
	I	Input voltage vs. output voltage ratio: logical value ± 5 %


\*1 Current measurements may not be stable due to the effects of the power supply line waveform or the wiring environment between the product and the EUT.




- Measurement circuit network  
(NetworkA IEC 60990 Fig. 3 U1 measurement)




- Measurement circuit network  
(NetworkB-U1 IEC 60990 Fig. 4 U2 measurement)

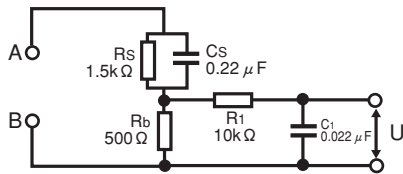


- Measurement circuit network  
(NetworkB-U2 IEC 60990 Fig. 4 U1 measurement)

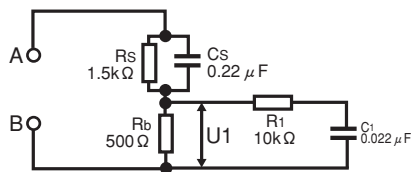


- Measurement circuit network  
(NetworkC IEC 60990 Fig. 5 U3 measurement)

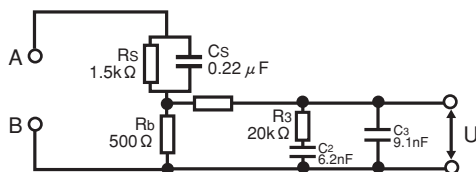


- Measurement circuit network  
(NetworkD Electrical Appliances and Materials Safety Act single frequency)




- Measurement circuit network  
(NetworkE Electrical Appliances and Materials Safety Act multiple frequencies)

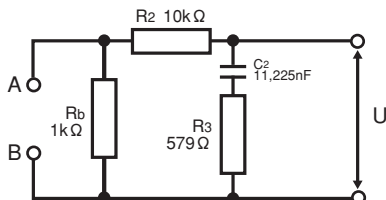


- Measurement circuit network  
(NetworkF IEC 61029, UL)




- Measurement circuit network  
(NetworkG IEC 60745)




- Measurement circuit network  
(NetworkI IEC 60601-1)



- Measurement circuit network  
(NetworkPCC-1)



- Measurement circuit network  
(NetworkPCC-2 IEC60598-1)



# Specifications

[Measurement section] The range varies by network.

Item			TOS9303LC	
Measurement range *1	Range 1		DC, RMS: 1.00 μA(min.) to 200.00 μA(max), Peak: 1.00 μA(min.) to 282.00 μA(max)	
	Range 2		DC, RMS: 12.50 μA(min.) to 2000.0 μA(max), Peak: 17.50 μA(min.) to 2830.0 μA(max)	
	Range 3		DC, RMS: 125.0 μA(min.) to 20.000 mA(max), Peak: 175.0 μA(min.) to 28.300 mA(max)	
	Range 4		DC, RMS: 1.250 mA(min.) to 100.00 mA(max), Peak: 1.750 mA(min.) to 100.00 mA(max)	
	Range switching		Auto or Fix selectable. If a measurement falls outside the measurement range of each range, the measured value blinks as a warning.	
	Auto		The range is set automatically according to the measurements.	
	Fix		For TC and PCC measurements, the measurement range is selected automatically according to the UPPER value. For meter measurements, the range is fixed to the specified range.	
	Bandwidth switching		Can be expanded to a bandwidth that allows measurements from 0.1 Hz, which is required in the measurement of medical instruments and the like.	
Normal		Normal measurement bandwidth: 15 Hz to 1 MHz		
Expand		Expands the measurement range to 0.1 Hz to 1 MHz		
Total accuracy *2 (when network A, B, or C is used) *3	Range 1	DC	±(5.0 % of reading + 2 μA)	
		RMS	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 2 μA)
			15 Hz ≤ f ≤ 100 kHz	±(7.0 % of reading + 2 μA)
			100 kHz < f ≤ 1 MHz	±(10.0 % of reading + 2 μA)
		Peak	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 10 μA)
			15 Hz ≤ f ≤ 1 kHz	±(10.0 % of reading + 10 μA)
			1 kHz < f ≤ 100 kHz	±(10.0 % of reading + 10 μA)
	Range 2	DC	±(5.0 % of reading + 20 μA)	
		RMS	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 10 μA)
			15 Hz ≤ f ≤ 100 kHz	±(7.0 % of reading + 8 μA)
			100 kHz < f ≤ 1 MHz	±(10.0 % of reading + 10 μA)
		Peak	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 10 μA)
			15 Hz ≤ f ≤ 1 kHz	±(10.0 % of reading + 10 μA)
			1 kHz < f ≤ 100 kHz	±(10.0 % of reading + 10 μA)
	Range 3	DC	±(5.0 % of reading + 50 μA)	
		RMS	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 20 μA)
			15 Hz ≤ f ≤ 100 kHz	±(7.0 % of reading + 20 μA)
			100 kHz < f ≤ 1 MHz	±(10.0 % of reading + 20 μA)
		Peak	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 50 μA)
			15 Hz ≤ f ≤ 1 kHz	±(7.0 % of reading + 50 μA)
			1 kHz < f ≤ 100 kHz	±(10.0 % of reading + 50 μA)
	Range 4	DC	±(5.0 % of reading + 0.5 mA)	
		RMS	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 0.2 mA)
			15 Hz ≤ f ≤ 100 kHz	±(7.0 % of reading + 0.2 mA)
			100 kHz < f ≤ 1 MHz	±(10.0 % of reading + 0.2 mA)
		Peak	0.1 Hz ≤ f < 15 Hz	±(10.0 % of reading + 0.5 mA)
			15 Hz ≤ f ≤ 1 kHz	±(7.0 % of reading + 0.5 mA)
			1 kHz < f ≤ 100 kHz	±(10.0 % of reading + 0.5 mA)
Input resistance			1 MΩ ± 1 %	
Input capacitance			200 pF or less (internal voltmeter input capacitance: 100 pF or less)	
Common mode rejection ratio			10 kHz or less: 60 dB or more, 10 kHz to 1 MHz: 40 dB or more	
Offset cancel function			Cancels up to 10 mA of the unnecessary current from measurements. OFF function available.	

\*1 Voltmeter band expansion is possible when network I is selected.

\*2 0.1 Hz  $\leq f < 15$  Hz is for when voltmeter band expansion (VoltMeter BandWidth) is set to Expand. Requires at least 120 second of test time.

\*3 A value converted to current for measurements using Network A, B, C or H with voltmeter accuracy of this product as the reference.

If a network other than A, B, C or H is used, calculate as follows:

For Network D, E, or I, the  $\blacksquare$  part of  $\pm(\square\% \text{ of reading} + \blacksquare\text{A})$  is half the value.

For F, the  $\blacksquare$  part is one-third the value.

For G, the  $\blacksquare$  part is one-fourth the value.

For PCC-1 or PCC-2, the  $\blacksquare$  part is 3.3 times the value.

### [Judgment function] The range varies by network.

Item			TOS9303LC
Behavior based on judgment	UPPER FAIL	Judgment method	Judgment starts after the judgment delay (Judge Delay). Buzzer volume level can be set in the range of 0 (OFF) to 10 for pass and fail separately. In an auto test, the buzzer is valid only for the judgment that takes place at the end of the program.
		Display	"Upper-FAIL" is displayed.
		Buzzer	On
		SIGNAL I/O	The Upper-FAIL signal is generated continuously until a STOP signal is received.
	LOWER FAIL	Judgment method	LOWER FAIL results when a current less than or equal to the lower limit (Lower) is detected.
		Display	"Lower-FAIL" is displayed.
		Buzzer	On
		SIGNAL I/O	The Lower-FAIL signal is generated continuously until a STOP signal is received.
	PASS	Judgment method	PASS judgment is made if Upper-FAIL or Lower-FAIL has not occurred when the test time elapses.
		Display	"PASS" is displayed.
		Buzzer	On (fixed to 50 ms)
		SIGNAL I/O	The PASS signal is generated for the length of time specified by the Pass Hold setting. If Pass Hold is set to Infinity, the PASS signal is generated continuously until a STOP signal is received.
Upper Setting range	RANGE 1		DC, RMS: 0.1 $\mu$ A(min.) to 200 $\mu$ A(max), Peak: 0.1 $\mu$ A(min.) to 282 $\mu$ A(max)
	RANGE 2		DC, RMS: 15.1 $\mu$ A(min.) to 2.00 mA(max), Peak: 21.3 $\mu$ A(min.) to 2.83 mA(max)
	RANGE 3		DC, RMS: 151 $\mu$ A(min.) to 20.00 mA(max), Peak: 213 $\mu$ A(min.) to 28.3 mA(max)
	RANGE 4		DC, RMS: 1.51 mA(min.) to 100 mA(max), Peak: 2.13 mA(min.) to 100 mA(max)
Lower Setting range			A value that is -1 digit from the upper setting range.
Judgment accuracy			Conforms to total accuracy(Read "reading" as "upper setting" of total accuracy.)

### [Timer function]

Item			TOS9303LC
Judgment delay (Judge Delay)	Setting range		1 s to 1000 s, OFF
	Accuracy		$\pm$ (100 ppm of setting + 20 ms)
Test time	Setting range		1 s to 1000 s, OFF
	Accuracy		$\pm$ (100 ppm of setting + 20 ms)

### [Other specifications]

Item			TOS9303LC
Voltage conversion			Displays the estimated current converted with the preset supply voltage (Conv Voltage), based on the voltage supplied to the EUT and the measured current. (This is invalid in meter mode.)
	Setting range		80.0 V to 300.0 V, OFF
	Resolution		0.1 V
Power supply line polarity selection			Set the polarity of the power supply line to supply to the EUT to positive or negative.
Single fault mode (Condition) selection			Set the EUT single fault mode to normal, neutral line disconnection (Fault Neu), or protective ground wire disconnection (Fault PE).
Ground check			In the touch current test between the enclosure and power supply line, if the EUT enclosure is grounded, Contact-FAIL occurs.
Measurement check			Checks the measurement function by shorting across the A and B terminals. If an error is found, the protection function is activated.
Supply voltage measurementAC LINE (EUT)	Measurement range		80.0 V to 250.0 V
	Resolution		0.01 V
	Accuracy		$\pm$ (3 % of reading + 1 V)
	Measurement range		0.1 A to 15.00 A
Supply current measurementAC LINE (EUT)	Resolution		0.001 A
	Accuracy		$\pm$ (5 % of reading + 30 mA)
	Measurement range		10 W to 1500 W
	Accuracy		$\pm$ (5 % of reading + 8 W) (with the supply voltage at 80 V or more, at a load power factor of 1)
Voltage measurement across the A and B terminals	Measurement range	DC	10.00 V to 300.0 V
		RMS	10.00 V to 300.0 V
		Peak	15.00 V to 430.0 V
		Input impedance	Approx. 40 M $\Omega$
	Accuracy *1		$\pm$ (3 % of reading + 2 V) (measurement range fixed to AUTO)
	SELV detection		Set a voltage for detecting SELV. When the value is exceeded, the DANGER LED lights.
		Setting range	10.0 V to 99.9 V, OFF
		Resolution	0.1 V
	Rated voltage	Between the A and B terminals	250 V
		Between the terminals and chassis	250 V
Measurement terminal	Rated current		100 mA
	Measurement category		CAT-II
	Valid terminal display		Terminals valid for measurement are indicated on the display.
	110% terminal		Terminal for supplying 110% voltage of the AC line.
	Nominal voltage range		100 V to 240 V, 50 Hz/60 Hz
Power supply for the EUT	Input voltage range (allowable voltage range)		85 Vac to 250 Vac
	Rated output capacity		1500 VA
	Maximum operating current		15 A (Overcurrent protection is activated at approximately 15.7 A.)
	Inrush current		70 Apeak max. (within 20 ms)



# Specifications

## ■ Interface (Common)

Item			TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
REMOTE			MINI DIN 9-pin connector. Connect the following option to remotely control the starting and stopping of tests. • Remote control box RC01-TOS, RC02-TOS • High voltage test probe HP01A-TOS, HP02A-TOS (when the test voltage is 4 kVac 5 kVdc or less)					
SIGNAL I/O			D-sub 37-pin connector. For the pin arrangement					
	Function	Enable/disable interlock, recall setup memories, recall auto test programs, start/stop testing, monitor the test and voltage generation status, monitor the test status, monitor judgment results, monitor the step execution status of auto tests, monitor the activation status of protection functions						
	Input specifications	The input signals are all low-active control. The input terminal is pulled up to +12 V by a resistor. Leaving the input terminal open is equivalent to applying a high level signal.						
		High-level input voltage	11 V to 15 V					
		Low-level input voltage	0 V to 4 V					
		Low-level input current	-5 mA max.					
	Output specifications	Input time width	5 ms min.					
		Output method	Open collector output (4.5 Vdc to 30 Vdc)					
		Output withstanding voltage	30 Vdc					
		Output saturation voltage	Approx. 1.1 V (25 °C)					
Maximum output current	400 mA(TOTAL)							
STATUS OUT			Output terminal of an option product.					
	Positive terminal (red)	Outputs +24 V. Use Status Out of CONFIG settings to set the output conditions.						
	Negative terminal (black)	+24 V circuit common.						
SCANNER			MINI DIN 8-pin connector. Terminal for the optional TOS9320 high voltage scanner. The maximum number of connections is 4 devices(16 channels).					
USB (host)			Standard type A socket, FAT32, 32 GB or less Complies with the USB 2.0 specifications; data rate: 12 Mbps (full speed)					
Remote control			All functions except turning on and off the power, key lock, and auto test can be remotely controlled.					
	RS232C	Hardware	D-sub 9-pin connector (EIA-232D compliant) Baud rate: 9600, 19200, 38400, 57600, 115200 bps Data length: 8 bits; stop bits: 1 bit; parity bit: none, flow control: none/CTS-RTS					
		Message terminator	LF during reception, LF during transmission.					
	USB (device)	Hardware	Standard Type B connector. Complies with the USB 2.0 specifications; data rate: 480 Mbps (high speed)					
		Message terminator	LF or EOM during reception, LF + EOM during transmission.					
	LAN	Device class	Complies with the USBTMC-USB488 device class specifications.					
		Hardware	IEEE 802.3 100Base-TX/10Base-T Ethernet. Auto-MDIX compliant.IPv4, RJ-45 connector.					
		Compliant standards	LXI 1.4 Core Specification 2011					
		Communication protocol	VXI-11, HiSLIP, SCPI-RAW, SCPI-Telnet					
	Message terminator	VXI-11, HiSLIP: LF or END during reception, LF + END during transmission. SCPI-RAW: LF during reception, LF during transmission.						
Display			7-inch LCD					

## ■ Other Functions (Common)

Item		TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
Auto test		Auto execution by combining ACW, DCW, IR, and EC. For LC, a combination is possible only using TC, PCC, and Patient.					
Test condition memory	Setup memory	Up to 51 test conditions (ACW, DCW, IR, EC, PD, LC) can be saved.					
	Program memory	Up to 100 program (ACW, DCW, IR, EC, PD) combinations, each containing 100 steps, can be saved.					
	Program memory (LC)	Up to 100 program (TC, PCC, Patient) combinations, each containing 100 steps, can be saved.					
Test result memory		Records up to 1000 latest test result of independent tests and auto tests. These are cleared when the power is turned off. Test results can be saved in CSV format to a USB memory device.					
System clock		For recording the calibration time and test times					
	Recordable time	Up to year 2038					
	Calibration period setting	Displays a warning at power-on when the specified period passes. Select whether to activate a protection function or only display a warning in the display area when a warning occurs.					
Measurement display		Maximum and minimum measurements can be displayed.					
	Normal	Displays measurements during a test. Maximum and minimum values are not held.					
	Maximum and minimum value display	Displays the maximum current measurement for withstanding voltage (ACW/DCW) tests, the minimum resistance measurement for insulation resistance (IR) tests, the resistance measurement or voltage measurement for earth continuity (EC) tests.					
Test start method	Double Action	When you press STOP, "READY" is shown for 0.5 seconds. A test starts only when you press START within this period.					
	Momentary	Tests are only executed while the START switch is held down.					
	Start Long	A test starts only when the START switch is held down for at least 1 second.					
PASS judgment display time (Pass Hold)		Set the time to hold the pass judgment result display (0.05 s to 10.00 s) or hold it until STOP is pressed (Infinity).					
STOP signal disable (Fail Mode)		It is possible to set the instrument so that fail judgment results and PROTECTION mode cannot be released from a device connected to the SIGNAL I/O connector or REMOTE connector.					
Key lock		Lock the operation of the keys to prevent changing the settings or overwriting memory or programs by mistake.					

## ■ Other Functions (Common)

Item	TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
Protection functions	If a protection function is activated during a test, the output is shut off and the test is stopped immediately. In an LC test, the power supply to the EUT is stopped, and the A and B terminals are opened. Conditions that cause a protection function to be activated are as follows.					
Interlock	Interlock is activated.					
Power Supply	There is an error in the power supply section.					
Output Error	An output voltage outside of the following range is detected. ACW, DCW, IR test, PD test: $\pm(10\% \text{ of setting} + 50 \text{ V})$ EC test: $\pm(10\% \text{ of setting} + 2 \text{ A})$					
Over Load	An output power or output current outside of the following range is detected. ACW: 550 VA, DCW: 110 W or 50 mA, IR (7200 V test): 110 W or 25 mA, IR (-1000 V test): 2 mA, EC: 240 VA, LC: AC LINE OUT current at approx. 15.7 A or power at 1600 VA.					
Over Heat	The internal temperature of the product is abnormally high.					
Over Rating	During a withstanding voltage test, an output current is generated for a length of time that exceeds the output time limit.					
Cal	The preset calibration period is exceeded.					
Remote	The REMOTE connector is connected or disconnected.					
Signal I/O	There is a change in the SIGNAL I/O connector's ENABLE signal.					
Communication	An internal communication error is occurring.					
Over Range	A value exceeding the maximum value of the measurement range is detected.					
Measure	An error is detected in the LC test measurement check.					
Short	A relay operation error is detected in an LC test.					
Earth Fault	When the grounding mode (GND) is set to Guard, abnormal current flows from the high voltage output of this product to ground.					
Scan I/F	While scanning, the interface cable is disconnected. Or, the channel-assigned scanner is not detected.					

## ■ General Specifications (Common)

Item			TOS9300	TOS9301	TOS9301PD	TOS9302	TOS9303	TOS9303LC
Backup battery life			3 years (at 25 °C)					
Environment	Installation location		Indoors, 2000 m or less					
	Spec guaranteed range	Temperature	5 °C to 35 °C (41 °F to 95 °F)(18 °C to 28 °C for partial discharge tests)					
		Humidity	20 %rh to 80 %rh (20 %rh to 70 %rh for partial discharge tests)(no condensation)					
	Operating range	Temperature	0 °C to 40 °C (32 °F to 104 °F)					
		Humidity	20 %rh to 80 %rh (no condensation)					
	Storage range	Temperature	-20 °C to 70 °C (-4 °F to 158 °F)					
Humidity		90 %rh or less (no condensation)						
Power supply	Nominal voltage range (allowable voltage range)		100 Vac to 120 V, 200 V to 240 V (90 Vac to 132 V, 170 V to 250 V)					
	Power consumption	No load(READY state)	100 VA or less					
		Rated load	800 VA max.					
	Allowable frequency range		47 Hz to 63 Hz					
Insulation resistance (between AC LINE and chassis)			30 MΩ or more (500 Vdc)					
Withstanding voltage (between AC LINE and chassis)			1500 Vac, 1 minute, 20 mA or less					
Earth continuity			25 Aac, 0.1 Ω or less					
Weight			TOS9300:Approx. 17 kg (37.5lb.), TOS9301:Approx. 18 kg (39.7lb.), TOS9301PD:22 kg (48.5lb.), TOS9302:Approx. 20 kg (44.1lb.), TOS9303:Approx. 21 kg (46.3lb.), TOS9303LC:Approx. 22 kg (48.5lb.)					
Accessories			Power cord (1 pc., *length: 2.5 m : The attached power cord varies depending on the shipment destination.), High-voltage test lead: TL31-TOS (1 pair), SIGNAL I/O plug (1 set), High-voltage warning sticker (1 pc.), Setup Guide (1 copy), CD-ROM (1 disc), Safety Information (1 copy), Heavy object warning label (1 pc., *Not included with the TOS9300), Test leads for earth continuity test: TL13-TOS (1 pair., *TOS9302, TOS9303,TOS9303LC only), [TOS9303LC only: Spare fuse (1 pc.), Test leads for leakage current test (2 red, 1 black), Flat probe (1 sheet)]					
Electromagnetic compatibility *1 *2			Complies with the requirements of the following directive and standards. EMC Directive 2014/30/EU EN 61326-1 (Class A *3), EN 55011 (Class A *3, Group 1 *4), EN 61000-3-2, EN 61000-3-3 Applicable under the following conditions The maximum length of all cabling and wiring connected to the product must be less than 2.5 m.Shielded cables are being used when using the SIGNAL I/O.The high-voltage test lead TL31-TOS is in use.Electrical discharges are applied only to the EUT.					
Safety *1			Complies with the requirements of the following directive and standards. Low Voltage Directive 2014/35/EU *2, EN 61010-1 (Class I *5 , Pollution Degree 2 *6)					

\*1 Does not apply to specially ordered or modified products.

\*2 Only on models that have CE/UKCA marking on the panel.

\*3 This is a Class A instrument. This product is intended for use in an industrial environment. This product may cause interference if used in residential areas. Such use must be avoided unless the user takes special measures to reduce electromagnetic emissions to prevent interference to the reception of radio and television broadcasts.

\*4 This is a Group 1 instrument. This product does not generate and/or use intentionally radio-frequency energy, in the form of electromagnetic radiation, inductive and/or capacitive coupling, for the treatment of material or inspection/analysis purpose.

\*5 This is a Class I instrument. Be sure to ground this product's protective conductor terminal. The safety of this product is guaranteed only when the product is properly grounded.

\*6 Pollution is addition of foreign matter (solid, liquid or gaseous) that may produce a reduction of dielectric strength or surface resistivity. Pollution Degree 2 assumes that only non-conductive pollution will occur except for an occasional temporary conductivity caused by condensation.

# Specifications

## ■ High Voltage Scanner

### [Basic specifications]

Item		TOS9320
Maximum operating voltage	AC	5 kV
	DC	7.2 kV
Number of channels		4 (Each channel can be set to high, low, or open.)
Maximum connections		4 units Channel numbers are assigned according to the order in which connections are made to the TOS9300 series tester. 1st scanner: CH1 to CH4, 2nd scanner: CH5 to CH8, 3rd scanner: CH9 to CH12, 4th scanner: CH13 to CH16
Contact check function		Available
Indicators	DANGER	Lights up in sync with the TOS9300 series tester
	CHANNEL	Indicates the setting of each channel with color. Red: High, Green: Low, Orange: Contact being checked, Off: Open
	EXTERNAL	Lights up when external control is on
	POWER	Lights up when the power is on

### [Interface and other functions]

Item		TOS9320	
Control switch		EXTERNAL I/O switch for switching the following controls. ON: External control through the CONTROLLER INTERFACE    OFF: Control from the TOS9300 series tester	
CONTROLLER INTERFACE (external control)		D-sub 25-pin connector.	
	Function		
	Sets each channel to high or low or all channels to open. Outputs the setting of each channel.		
	Input	The input signals are all low-active control. The input terminal is pulled up to +12 V by a resistor. Leaving the input terminal open is equivalent to applying a high level signal.	
		High-level input voltage	11 V to 15 V
		Low-level input voltage	0 V to 4 V
		Low-level input current	-5 mA max.
		Input time width	5 ms min.
	Output	Output method	Open collector output (4.5 Vdc to 30 Vdc)
		Output withstanding voltage	30 Vdc
		Output saturation voltage	Approx. 1.1 V (25°C, 77°F)
Maximum output current		400 mA (TOTAL)	
TOS9300 series tester interface		MINI DIN 8-pin connector. Accuracy guaranteed up to 4 units (16 channels)	

### [General specifications]

Item		TOS9320
Environment	Installation location	Indoors, 2000 m or less
	Spec guaranteed range	Temperature 5°C to 35°C (41°F to 95°F)
		Humidity 20%rh to 70%rh (no condensation)
	Operating range	Temperature 0°C to 40°C (32°F to 104°F)
		Humidity 20%rh to 80%rh (no condensation)
	Storage range	Temperature -20°C to 70°C (-4°F to 158°F)
		Humidity 90%rh or less (no condensation)
Power supply	Nominal voltage range (allowable voltage range)	100 Vac to 240 Vac (90 Vac to 250 Vac)
	Power consumption	50 VA max.
	Allowable frequency range	47 Hz to 63 Hz
Insulation resistance (between AC LINE and chassis)		30 MΩ or more (500 Vdc)
Withstanding voltage (between AC LINE and chassis)		1500 Vac for 1 minute, 20 mA or less
Earth continuity		25 Aac/0.1 Ω or less
Weight		Approx. 8 kg (17.6 lb)
Accessories		Power cord (1 pc., length: 2.5 m: The attached power cord varies depending on the shipment destination.) High-voltage test lead [TL31-TOS] (8 red), Lead for high voltage parallel connection TL33-TOS (1 pair), Interface cable (1 pc.), CONTROLLER INTERFACE plug (1 set), High-voltage warning sticker (2 pc.), Channel labels (For the panel (1 sheet), For the test leads (1 sheet)), User's manual (1 copy), Safety Information (1 copy)
Electromagnetic compatibility *1 *2		Complies with the requirements of the following directive and standards. EMC Directive 2014/30/EU, EN 61326-1 (Class A *3), EN 55011 (Class A *3, Group 1 *4), EN 61000-3-2, EN 61000-3-3 Applicable under the following conditions The maximum length of all cabling and wiring connected to this product is less than 2.5 m. A shielded cable is used for the connection to the CONTROLLER INTERFACE. The high-voltage test lead TL31-TOS is in use. Electrical discharges are applied only to the EUT.
Safety *1		Complies with the requirements of the following directive and standards. Low Voltage Directive 2014/35/EU *2, EN 61010-1 (Class I *5, Pollution Degree 2 *6)

\*1 Does not apply to specially ordered or modified products.

\*2 Only on models that have CE/UKCA marking on the panel.

\*3 This is a Class A instrument. This product is intended for use in an industrial environment. This product may cause interference if used in residential areas. Such use must be avoided unless the user takes special measures to reduce electromagnetic emissions to prevent interference to the reception of radio and television broadcasts.

\*4 This is a Group 1 instrument. This product does not generate and/or use intentionally radio-frequency energy, in the form of electromagnetic radiation, inductive and/or capacitive coupling, for the treatment of material or inspection/analysis purpose.


\*5 This is a Class I instrument. Be sure to ground this product's protective conductor terminal. The safety of this product is guaranteed only when the product is properly grounded.

\*6 Pollution is addition of foreign matter (solid, liquid or gaseous) that may produce a reduction of dielectric strength or surface resistivity. Pollution Degree 2 assumes that only non-conductive pollution will occur except for an occasional temporary conductivity caused by condensation.




# External Dimensions (Unit:mm(inches))


**TOS9300** **TOS9301**

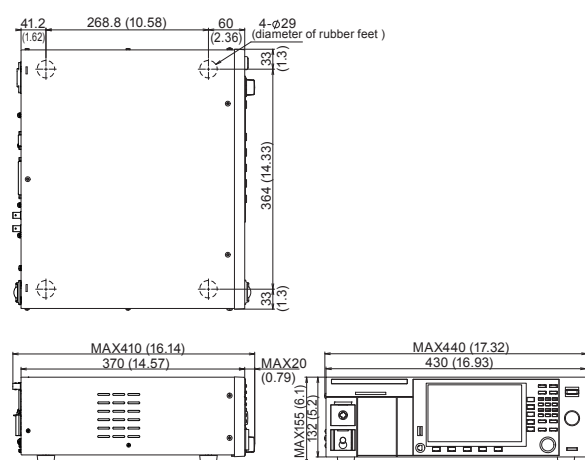


**TOS9303LC**

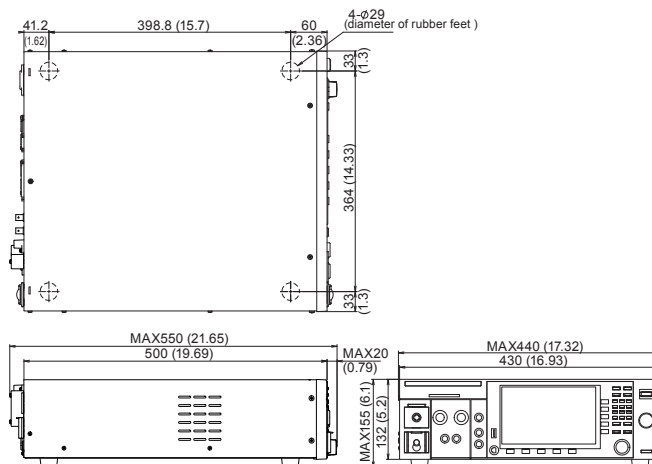


**TOS9301PD**

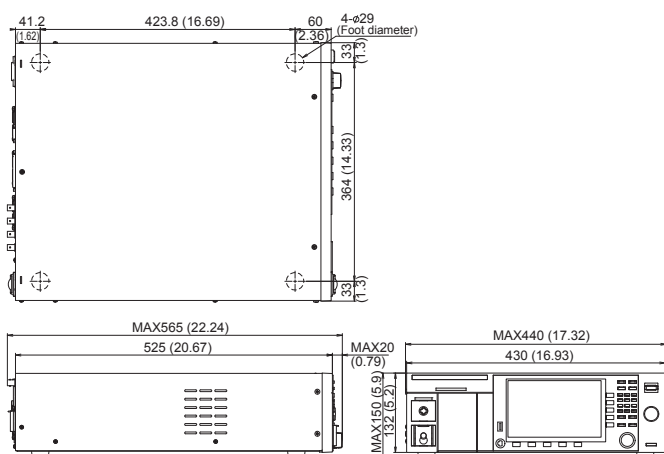

**TOS9320**

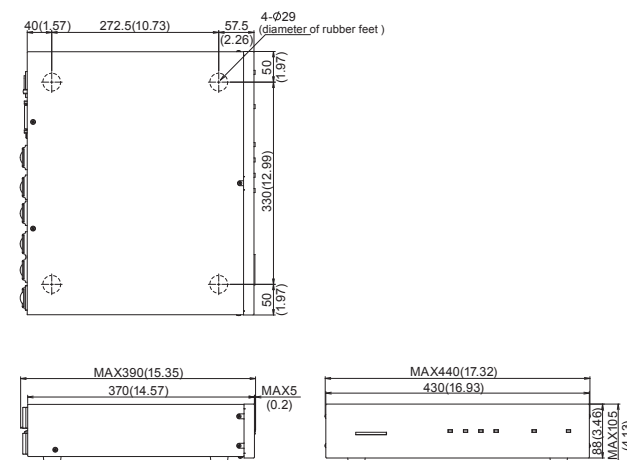

**TOS9302** **TOS9303**

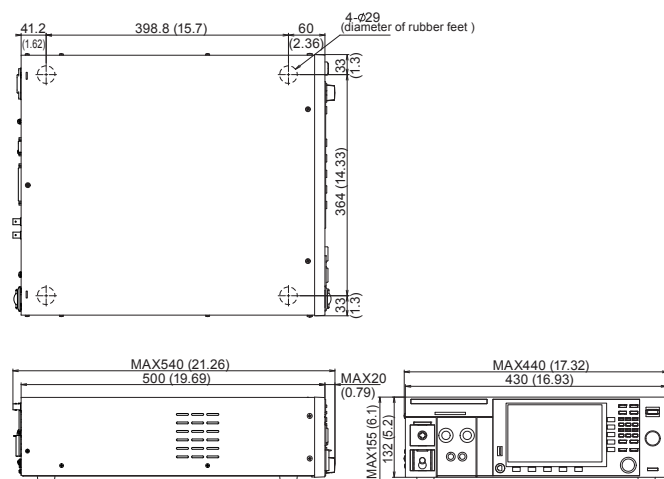

## Option

### High-Voltage Scanner

#### TOS9320



#### Dimensions(Maximum) / Weight

430(16.93") (440(17.32")) W × 88(3.46") (105(4.13")) H ×  
370(14.57") (390(15.35")) D mm / 8 kg(17.6 lbs)

## High-Voltage Scanner for TOS9300 Series for Multi-Channel Testing Systems

The high-voltage scanner TOS9320 is a specialized option for the TOS9300 series, capable of rapidly distributing test voltage from the main unit to multiple testing points for withstanding voltage and insulation resistance testing. Channels can be controlled with an external device through the back panel CONTROLLER INTERFACE connector. Remote control is not limited to the TOS9300 series, but is also compatible with previous models such as the TOS5300 series hipot/insulation resistance tester. The TOS9320 high-voltage scanner is an essential tool for the automation of highly reliable testing of electronic devices among multiple channels.

#### Features

- Output can be expanded to four channels with one high-voltage scanner. The electric potential of each channel can be arbitrarily set to high, low, or open, and can be tested at any of these four points.
- Up to four high voltage scanners (total 16 channels) can be connected to each unit.
- Output of each channel and contact with testing points can be easily monitored.

### Remote Control Box

The remote control box can be used to start and stop withstanding voltage and insulation resistance tests. One model is for use with one hand, and the other model is for use with two hands.

#### RC01-TOS (One-hand operation/1.5 m)



\*DD-5P/9P DIN conversion cable required for connection with TOS9300 series.

#### RC02-TOS (Two-hand operation/1.5 m)



\*DD-5P/9P DIN conversion cable required for connection with TOS9300 series.

### DIN Conversion Cable

The DIN (5 pin → 9 pin) conversion cable is used for connection with the following optional products and the TOS9300 series.

- Remote control box(RC01-TOS/RC02-TOS)
- High voltage test probe(HP01A-TOS/HP02A-TOS)

#### DD-5P/9P Adaptor/DIN to Mini DIN



### Warning Light Unit

The warning light unit indicates when the TOS9300 is performing a test, making clear that a test is in progress from a distance.

#### PL02A-TOS (for DC24 V)



### Multi Outlet

The multi outlet OT01-TOS can be used to connect to main plug standards world wide by connecting to the AC LINE OUT terminal block of the EUT power supply

#### OT01-TOS

for TOS9303LC



### High-Voltage Test Probe

This probe is used for generating test voltage. This probe has been designed to only generate test voltage when the user operates the probe with both hands in order to prevent accidental test voltage generation.





#### HP01A-TOS (Max.AC4 kV • DC5 kV/1.8 m)

#### HP02A-TOS (Max.AC4 kV • DC5 kV/3.5 m)



\*DD-5P/9P DIN conversion cable required for connection with TOS9300 series.

### Rack Mount Bracket

Complied Model	JIS Standard	EIA Standard
	Bracket Model Name	Bracket Model Name
TOS9300 TOS9301 TOS9301PD TOS9302 TOS9303 TOS9303LC	KRB150-TOS	KRB3-TOS
		
TOS9320	KRB100-TOS	KRB2-TOS
		

### High-Voltage Digital Voltmeter

- Measurement of high voltages (AC/DC) of up to 10 kV maximum
- Large 4 1/2 digit LED display
- High measuring accuracy and input resistance
- Light weight of only 3 kg
- Compact design
- Excellent ease of maintenance

■ 149-10A



Specification	
Type	Double integration type. (sampling cycle: 3 times/sec)
DC Voltage	Measuring range: 0.500 kV to 10,000 kV Accuracy: $\pm(0.5\% \text{ of reading} + 0.03\% \text{ of range})$ Input resistance: $1000 \text{ M}\Omega \pm 2\%$
AC Voltage	Measuring range: 0.500 kV to 10,000 kV Accuracy: $\pm(1\% \text{ of reading} + 0.05\% \text{ of range})$ Frequency characteristics: 50/60 Hz (sine wave rms value display of mean value response) Input resistance: $1000 \text{ M}\Omega \pm 2\%$
Power	$100 \text{ V} \pm 10\%$ , Approx. 10 VA
Dimensions (MAX)	134[5.27 inch]W $\times$ 164[6.46 inch]H $\times$ 270[10.63 inch]D mm (140[5.51 inch]W $\times$ 189[7.44 inch]H $\times$ 350[13.78 inch]D mm)
Weight	Approx. 3 kg (6.6 lbs)
Accessories	TL05-TOS High voltage test leads: 1 HTL2.5DH High voltage test lead: 1

### UL Resistance Load

This device is described in section 125, paragraph 2-1B1 of UL1492. The RL01-TOS is a variable load resistor for checking the output voltage of hipot testers used in dielectric strength testing on production lines. (Complies with UL regulations including UL1270, UL1409 and UL1410.)

■ RL01-TOS



Specification	
Resistors	120 k $\Omega$ / 159 k $\Omega$ / 210 k $\Omega$ / 279 k $\Omega$ / 369 k $\Omega$ / 489 k $\Omega$ / 648 k $\Omega$ / 858 k $\Omega$ / 1,137 k $\Omega$ / 1,500 k $\Omega$ / 1,989 k $\Omega$ / 2,148 k $\Omega$
Resistance Accuracy	+1 %, -0 % of nominal value when set to 120 k $\Omega$ , $\pm 1\%$ of nominal value when set to other values
Maximum Operating Voltage	1300 V (continuous rating)
Maximum Overload Voltage	1400 V for 5 seconds (application may not be repeated within 1 minute)
Dimensions (MAX)	200[7.87 inch]W $\times$ 100[3.94 inch]H $\times$ 260[10.24 inch]D mm (210[8.27 inch]W $\times$ 120[4.72 inch]H $\times$ 295[11.61 inch]D mm)
Weight	Approx. 2.6 kg (5.73 lbs)
Accessories	TL04-TOS High-voltage test lead: 2 TL05-TOS High-voltage test lead: 1

### Calibration Resistor for Insulation Resistance Tester

The 929 Series Standard Resistors are for calibration of Insulation Testers.

- 929-1M (1 M $\Omega$ )
- 929-10M (10 M $\Omega$ )
- 929-100M (100 M $\Omega$ )









Specification	
Nominal Resistance	1 M $\Omega$ (929-1M)/ 10 M $\Omega$ (929-10M) 100 M $\Omega$ (929-100M)
Accuracy of Resistance	1 % at 25 °C $\pm 10$ °C
Temperature Coefficient	100 ppm/°C or better
Voltage Coefficient	1 ppm/V or better
Working voltage rating	1.2 kV
Dimensions (MAX)	64[25.20 inch]W $\times$ 24[9.45 inch]H $\times$ 30[11.81 inch]D mm

\*The 929 series standard resistors can not be installed directly to the TOS series. Please use the test lead for connection.

# Lineup Overview

## ●Electrical Safety Multi-analyzer

Model	Test items					
	 AC Withstanding Voltage (AC Hipot)	 DC Withstanding Voltage (DC Hipot)	 Insulation Resistance	 Earth Continuity (Ground Bond)	 Leakage Current	 Partial Discharge
<b>TOS9300</b>	●		●			
<b>TOS9301</b>	●	●	●			
<b>TOS9301PD</b> <span style="background-color: red; color: white; padding: 2px;">NEW</span>	●	●	●			●
<b>TOS9302</b>	●			●		
<b>TOS9303</b>	●	●	●	●		
<b>TOS9303LC</b>	●	●	●	●	●	

## ●Option

Description	Model	Remark
High-voltage scanner	<b>TOS9320</b>	4 channel high-voltage scanner with contact check function; can be used standalone
Remote control box	<b>RC01-TOS</b>	One-hand operation/1.5 m
	<b>RC02-TOS</b>	Both-hands operation/1.5 m
DIN conversion cable	<b>DD-5P/9P</b>	It is required when RC01-TOS/RC02-TOS, HP01A-TOS/HP02A-TOS and HP21-TOS is used
High-voltage test probe	<b>HP01A-TOS</b>	Max.AC4 kV • DC5 kV/1.8 m
	<b>HP02A-TOS</b>	Max.AC4 kV • DC5 kV/3.5 m
Warning light unit	<b>PL02A-TOS</b>	for DC24 V
Multi outlet	<b>OT01-TOS</b>	for TOS9303LC
Rack mount bracket	<b>KRB150-TOS</b>	JIS standard (mm) for TOS9300/9301/9301PD/9302/9303/9303LC
	<b>KRB3-TOS</b>	EIA standard (inch) for TOS9300/9301/9301PD/9302/9303/9303LC
	<b>KRB100-TOS</b>	JIS standard (mm) for TOS9320
	<b>KRB2-TOS</b>	EIA standard (inch) for TOS9320



### KIKUSUI ELECTRONICS CORPORATION

Southwood 4F,6-1 Chigasaki-chuo,Tsuzuki-ku,Yokohama,224-0032,Japan  
Phone: (+81)45-482-6353,Facsimile: (+81)45-482-6261,www.kikusui.co.jp

**KIKUSUI AMERICA, INC.** 1-310-214-0000 [www.kikusuiamerica.com](http://www.kikusuiamerica.com)



3625 Del Amo Blvd, Suite 160, Torrance, CA 90503  
Phone : 310-214-0000 Facsimile : 310-214-0014

**KIKUSUI TRADING (SHANGHAI) Co., Ltd.** [www.kikusui.cn](http://www.kikusui.cn)



Room 305,Shenggao Building ,No.137,Xianxia Road, Shanghai City, China  
Phone : 021-5887-9067 Facsimile : 021-5887-9069

## ● Distributor/Representative

■ All products contained in this catalogue are equipment and devices that are premised on use under the supervision of qualified personnel, and are not designed or produced for home-use or use by general consumers. ■ Specifications, design and so forth are subject to change without prior notice to improve the quality. ■ Product names and prices are subject to change and production may be discontinued when necessary. ■ Product names, company names and brand names contained in this catalogue represent the respective registered trade name or trade mark. ■ Colors, textures and so forth of photographs shown in this catalogue may differ from actual products due to a limited fidelity in printing. ■ Although every effort has been made to provide the information as accurate as possible for this catalogue, certain details have unavoidably been omitted due to limitations in space. ■ If you find any misprints or errors in this catalogue, it would be appreciated if you would inform us. ■ Please contact our distributors to confirm specifications.