

GRAS 46AK

1/2" CCP Free-field Standard Microphone Set



Freq range: 3.15 Hz to 20 kHz
Dyn range: 17 dB(A) to 138 dB
Sensitivity: 50 mV/Pa

The GRAS 46AK is a 1/2" Constant Current Power (CCP) free-field microphone set featuring a very short preamplifier for measurements in confined spaces.

GRAS Sound & Vibration
Skovlytoften 33, 2840 Holte, Denmark



ES France - Département Tests & Mesures
127 rue de Buzenval BP 26 - 92380 Garches



Tél. 01 47 95 99 45



e-mail : tem@es-france.com
Site Web : www.es-france.com

Introduction

The 46AK is a free-field microphone set and as such optimized for all acoustic applications, where the location of the main sound source is known and the microphone can be pointed directly at it ensuring 0° incidence.

The wide frequency range makes it ideal for general acoustic measurements. 46AK conforms with IEC 61094 WS2F and IEC 61672 Class 1.

A pressure version is available, 46A0-S2 1/2" CCP Pressure Microphone Set.

Design

The GRAS 46AK is a high-performance 1/2" free-field standard microphone set assembled in our clean-room environment and sealed with a label.

Microphone

The microphone cartridge is the high-quality IEC 61094 WS2F standardized [GRAS 40AE](#) 1/2" Prepolarized Free-field Microphone, designed for long-term reliability in multiple environments. The high sensitivity and reliability have made 40AE the preferred measurement microphone for sound level meters/analyzers with CCP-option and, as such, enables IEC 61672 Class 1 measurements.

Preamplifier

The preamplifier is the [GRAS 26CK](#) 1/2" CCP Standard Preamplifier with microdot connector and based on our well-known circuit board substrates. In the industry, these are known for their low self-noise, wide frequency, and excellent slew rate performance.

Compatibility

To perform as specified the GRAS 46AK microphone set requires a constant current input module that can deliver 4 mA and 24 V unloaded CCP voltage

supply. If the constant current supply is lower, the capability of driving long cables is reduced and consequently the upper frequency is reduced. If the voltage supply is lower it will influence the upper dynamic range.

The microphone set is terminated with a microdot 10/32 connector. Ready to use coax cable assemblies of various types and lengths are available in standard as well as customized lengths.

The 46AK is IEEE1451.4 TEDS v. 1.0 compliant. If your measurement platform supports Transducer Electronic Data Sheets you will be able to read and write data like properties and calibration data.

System verification

The functionality of TEDS is very useful to determine which microphone is connected to which input channel. However, it is not a check of whether the microphone is within specifications or not. For daily verification and check of your measurement setup, we therefore recommend using a sound source like the [GRAS 42AG](#) Sound Calibrator.

Calibration

When leaving the factory, all GRAS microphones have been calibrated in a controlled laboratory environment using traceable calibration equipment. Depending on the use, measurement environment and internal quality control programs we recommend that the microphone is recalibrated at least once a year.

We offer two kinds of calibration as an optional after-sales service: GRAS Traceable Calibration and GRAS Accredited Calibration.

GRAS Traceable Calibration is a traceable calibration performed by trained personnel under controlled conditions according to established procedures and standards. This is identical to the rigorous



calibration that all GRAS microphones are subjected to as an integral part of our quality assurance.

GRAS Accredited Calibration is performed by the GRAS Accredited Calibration Laboratory that has been accredited in accordance with ISO 17025 by DANAK, the Danish Accreditation Fund.

If you want a new microphone set delivered with an accredited calibration instead of the default factory calibration, specify this when ordering.

Learn more about [calibration](#) services on our website.

Quality and warranty

GRAS microphone sets are made of components from our proven standard portfolio and are all manufactured of high-quality material and branded parts that were chosen and processed to ensure life-long stability and robustness.

All parts are manufactured and assembled at the factory in Denmark by skilled and dedicated operators in a verified clean-room environment. The microphone diaphragm, body and unique protection grid are made of high-grade stainless steel and make the microphone set resistant to physical damage as well as corrosion caused by aggressive air or gases.

This, together with the enforced gold-plated microphone terminal guarantees a highly reliable connection. Thanks to the high quality, our warranty against defective materials and workmanship is 5 years.

Service

Should you accidentally damage the diaphragm on a GRAS microphone we will in most cases be able to exchange it at a very reasonable cost and short turn-around time. This not only protects your

investment but also supports your quality assurance processes department since you do not have to worry about new serial numbers etc.



Polarization/Connection		0 V / CCP
Frequency range (± 1 dB)	Hz	5 to 10 k
Frequency range (± 2 dB)	Hz	3.15 to 20 k
Dynamic range lower limit with GRAS preamplifier	dB(A)	17
Dynamic range upper limit with GRAS preamplifier	dB	138
Set sensitivity @ 250 Hz (± 1.5 dB)	mV/Pa	50
Set sensitivity @ 250 Hz (± 1.5 dB)	dB re 1V/Pa	-26
Output impedance	Ω	< 50
Output Voltage Swing, min. @ 24-28 V CCP voltage supply	V _p	8
Power supply min. to max.	mA	2 to 20
DC bias voltage, typ.	V	12
Microphone venting		Rear
IEC 61094-4 Designation		WS2F
Temperature range, operation	$^{\circ}\text{C} / ^{\circ}\text{F}$	-30 to 85 / -22 to 185*
Temperature range, storage	$^{\circ}\text{C} / ^{\circ}\text{F}$	-40 to 85 / -40 to 185
Temperature coefficient @250 Hz	dB/ $^{\circ}\text{C}$ / dB/ $^{\circ}\text{F}$	-0.01 / -0.006
Static pressure coefficient @250 Hz	dB/kPa	-0.007
Humidity range non condensing	% RH	0 to 90
Humidity coefficient @250 Hz	dB/% RH	-0.001
Influence of axial vibration @1 m/s ²	dB re 20 μPa	66
TEDS UDID (IEEE 1451.4)		I27-0-0-0U
Connector type		Microdot 10/32
CE/RoHS compliant/WEEE registered		Yes/Yes/Yes
Weight	g / oz	25 / 0.881


*If used at temperatures higher than 70 $^{\circ}\text{C}$, use high temperature cables.

Test conditions


Temperature: 20 $^{\circ}\text{C}$

Pressure: 760 mmHg



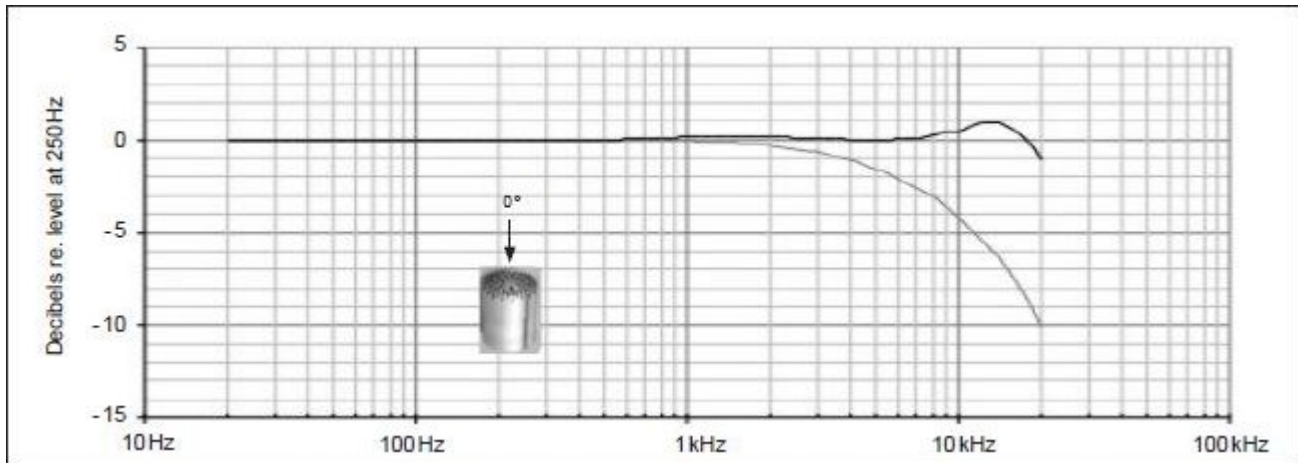


Typical frequency response. Upper curve shows free-field response for 0°, lower curve shows pressure response.

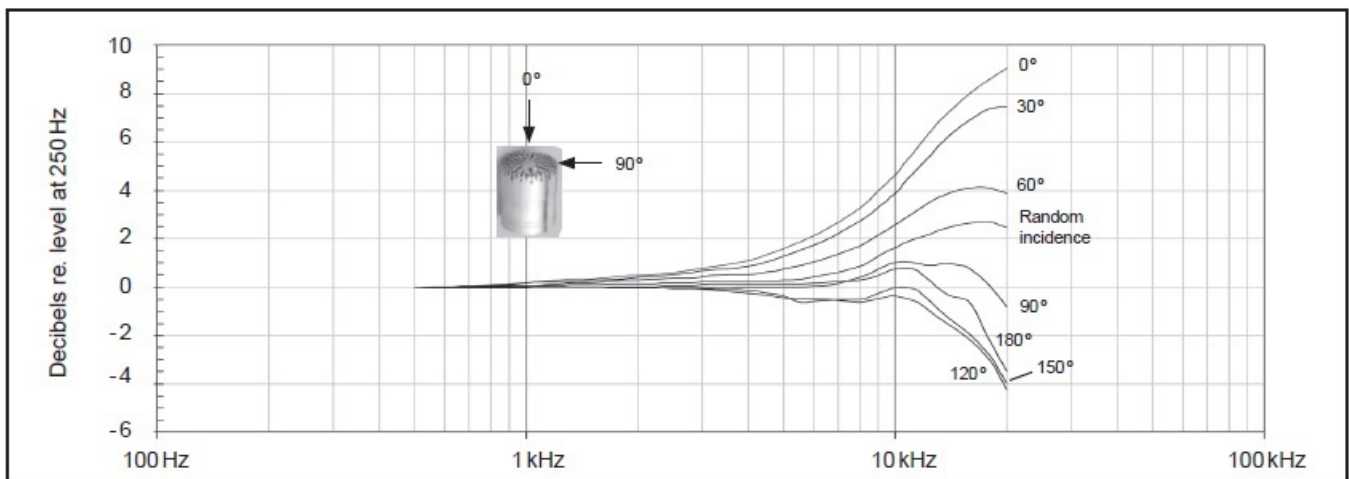

Free-field corrections for different angles of incidence

GRAS Sound & Vibration reserves the right to change specifications without notice.

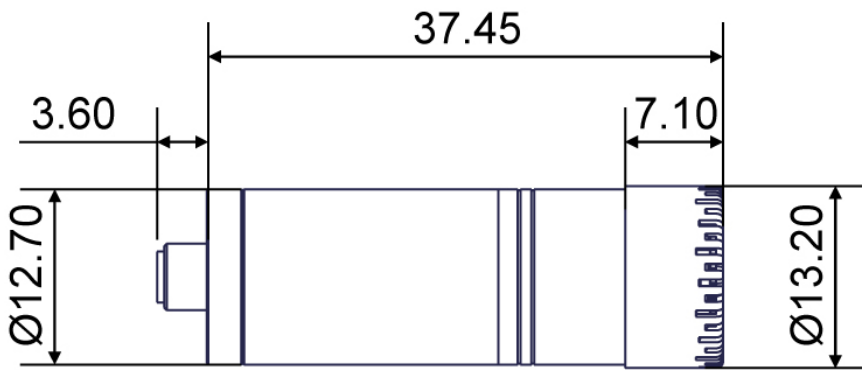

GRAS 46AK	1/2" CCP Free-field Microphone Set. This is the "standard" rear-vented version.
GRAS 46AK-FV	1/2" CCP Free-field Microphone Set, Front Vented. Identical to 46AK, but with front venting.

Optional items

GRAS RA0122	Random Incidence Corrector
GRAS AA0027	3 m Microdot - BNC Cable
GRAS AL0008	1/2" Microphone Holder, POM
GRAS AL0012	1/2" Microphone Holder, Stainless Steel
GRAS AL0005	Swivel head
GRAS AL0006	Tripod
GRAS RA0020	1/2" Nosecone
GRAS AM0069	Windscreen for 1/2" Microphones
GRAS RA0131	1/2" Rain protection cap
GRAS 12AL	1-Channel CCP Power Module with A-weighting filter
GRAS 12AQ	2-Channel Universal Power Module with signal conditioning and PC interface
GRAS 42AG	Multifunction Sound Calibrator, Class 1
GRAS 42AP	Intelligent Pistonphone, Class 0
GRAS CA0029	Traceable Calibration of Microphone Set
GRAS CA2301	Accredited Calibration of Microphone Set

GRAS Sound & Vibration reserves the right to change accessories without notice.

